
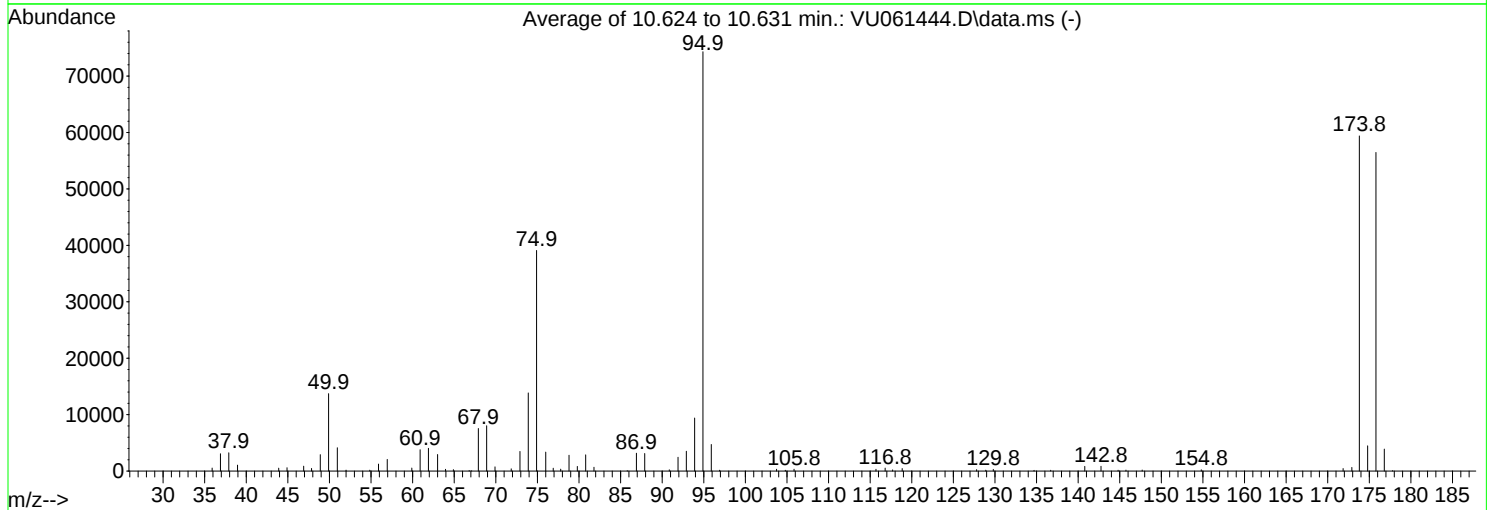


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110524\
Data File : VU061444.D
Acq On : 05 Nov 2024 09:10
Operator : MD/SY
Sample : BFB020
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 07 00:10:32 2024

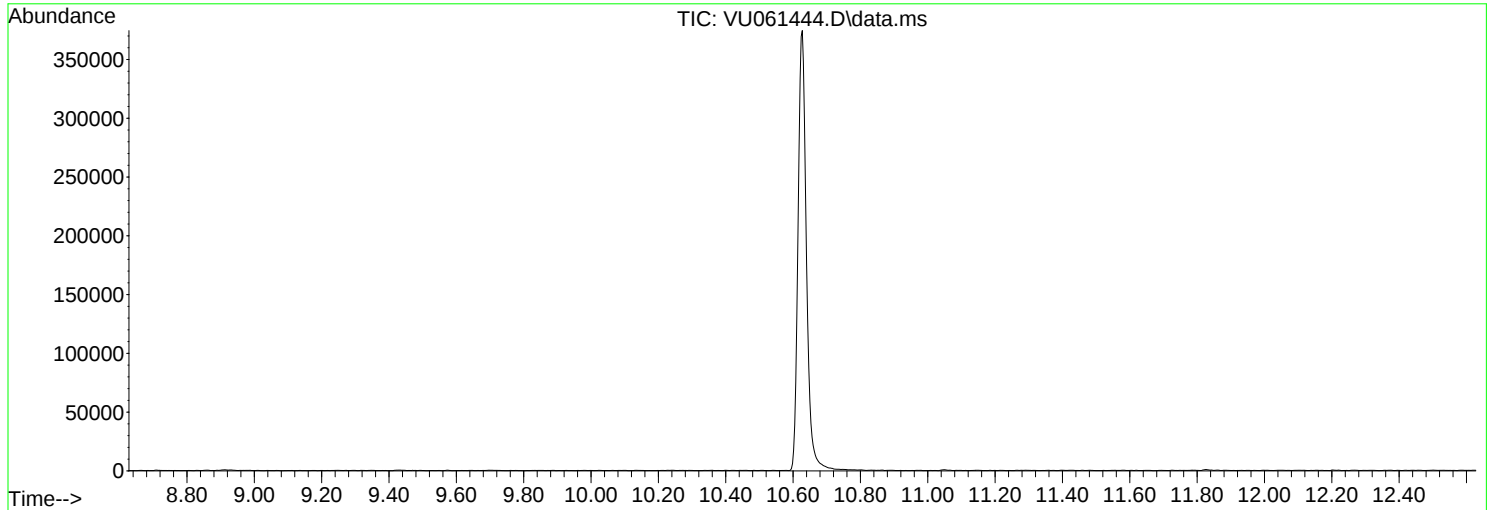

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	13726	PASS
75	95	30	80	52.6	39099	PASS
95	95	100	100	100.0	74317	PASS
96	95	5	9	6.3	4719	PASS
173	174	0.00	2	1.1	645	PASS
174	95	50	120	79.9	59397	PASS
175	174	5	9	7.5	4477	PASS
176	174	95	101	95.1	56464	PASS
177	176	5	9	6.9	3897	PASS

m/z	Abundance
39.90	112.0
44.00	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	601.0
36.90	3186.0
37.90	3321.0
38.90	1070.0
40.00	103.0
43.90	872.0
44.90	584.0
46.90	882.0
47.90	529.0
48.90	2996.0
49.90	14229.0
51.00	4105.0
52.00	201.0
54.90	166.0
55.90	1221.0
57.00	2032.0
59.90	561.0
60.90	3933.0
61.90	4079.0
63.00	3016.0
63.90	278.0
64.90	226.0
66.80	168.0
67.90	7802.0
68.90	8463.0
69.90	750.0
71.80	436.0
72.90	3726.0
73.90	14369.0
74.90	40008.0
76.00	3504.0
76.90	507.0
77.80	378.0
78.80	2832.0
79.80	805.0
80.80	2962.0
81.80	732.0
85.80	131.0
86.90	3137.0
87.90	3185.0
90.80	219.0
91.90	2424.0
92.90	3479.0
93.90	9634.0
94.90	75592.0
95.90	4953.0
96.90	153.0
103.80	371.0
104.80	120.0
105.80	361.0
115.70	319.0
116.80	500.0
117.70	228.0
118.90	530.0
127.80	244.0
128.90	162.0
129.80	276.0
134.70	116.0
136.70	160.0
140.80	893.0
142.70	861.0
144.80	151.0
145.80	164.0
147.70	200.0
154.80	235.0
171.80	527.0
172.90	636.0
173.80	59104.0
174.80	4511.0
175.80	56352.0
176.80	3777.0
177.80	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	544.0
36.90	3167.0
37.90	3345.0
38.90	1069.0
43.90	840.0
44.90	615.0
46.90	925.0
47.90	488.0
48.90	2979.0
49.90	14081.0
50.90	4276.0
52.00	179.0
54.80	163.0
55.90	1291.0
57.00	2102.0
59.90	539.0
60.90	3904.0
61.90	4198.0
63.00	3021.0
63.90	311.0
64.90	256.0
66.80	144.0
67.90	7722.0
68.90	8253.0
69.90	785.0
71.90	404.0
72.90	3548.0
73.90	14285.0
74.90	40264.0
76.00	3428.0
76.90	533.0
77.80	370.0
78.80	2851.0
79.80	859.0
80.80	2939.0
81.80	703.0
85.80	108.0
86.90	3292.0
87.90	3296.0
90.90	232.0
91.90	2551.0
92.90	3656.0
93.90	9673.0
94.90	76392.0
95.90	4812.0
96.90	165.0
103.80	323.0
104.80	150.0
105.90	329.0
115.70	343.0
116.80	523.0
117.70	211.0
118.90	439.0
127.80	269.0
128.90	173.0
129.80	304.0
134.70	123.0
136.70	151.0
140.80	850.0
142.80	868.0
144.80	162.0
145.70	192.0
147.70	200.0
154.80	242.0
171.80	446.0
172.90	669.0
173.80	61304.0
174.80	4649.0
175.80	57944.0
176.80	4010.0
177.80	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	472.0
36.90	2863.0
37.90	3065.0
39.00	1019.0
43.90	746.0
44.90	590.0
46.90	815.0
47.80	378.0
48.90	2765.0
49.90	12867.0
50.90	4031.0
52.00	136.0
54.80	173.0
55.90	1222.0
56.90	2066.0
59.90	529.0
60.90	3529.0
61.90	3823.0
63.00	2775.0
64.00	353.0
64.90	290.0
67.10	161.0
67.90	7107.0
68.90	7378.0
69.90	730.0
71.90	351.0
72.90	3165.0
73.90	12892.0
74.90	37024.0
76.00	3165.0
76.90	502.0
77.80	294.0
78.80	2736.0
79.80	819.0
80.80	2730.0
81.80	623.0
86.90	3072.0
87.90	2859.0
90.90	237.0
91.90	2378.0
92.90	3420.0
93.90	8908.0
94.90	70968.0
95.90	4393.0
96.90	157.0
103.70	278.0
104.80	168.0
105.90	308.0
115.70	313.0
116.80	560.0
117.70	219.0
118.70	376.0
127.80	246.0
128.90	151.0
129.80	311.0
134.70	146.0
136.70	127.0
140.80	770.0
142.80	829.0
144.80	150.0
145.70	194.0
147.70	167.0
154.80	206.0
171.90	374.0
172.90	630.0
173.80	57784.0
174.80	4272.0
175.80	55096.0
176.80	3903.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020