

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
 Data File : VU061493.D
 Acq On : 06 Nov 2024 11:38
 Operator : MD/SY
 Sample : P4714-19
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AJ9

Quant Time: Nov 07 00:50:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 07 00:10:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.241	114	151801	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	140662	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	62858	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	46939	4.552	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.000%
7) Chloroethane-d5	1.907	69	50432	5.335	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.600%
11) 1,1-Dichloroethene-d2	2.560	65	21752	4.930	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.600%
20) 2-Butanone-d5	4.624	46	106627	50.930	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.860%
24) Chloroform-d	5.052	84	99533	5.085	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	5.692	65	50790	5.206	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.717	84	203364	5.131	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
36) 1,2-Dichloropropane-d6	6.682	67	63642	5.341	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.800%
41) Toluene-d8	7.891	98	184414	4.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
43) trans-1,3-Dichloroprop...	8.174	79	19552	4.020	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.627	63	94564	47.467	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.940%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	46916	5.207	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	58722	5.276	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%
Target Compounds						
13) Acetone	2.644	43	6663	5.025	ug/L	90
16) Methylene chloride	3.039	84	33646	3.181	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061493.D
Acq On : 06 Nov 2024 11:38
Operator : MD/SY
Sample : P4714-19
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AJ9

Quant Time: Nov 07 00:50:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 07 00:10:32 2024
Response via : Initial Calibration

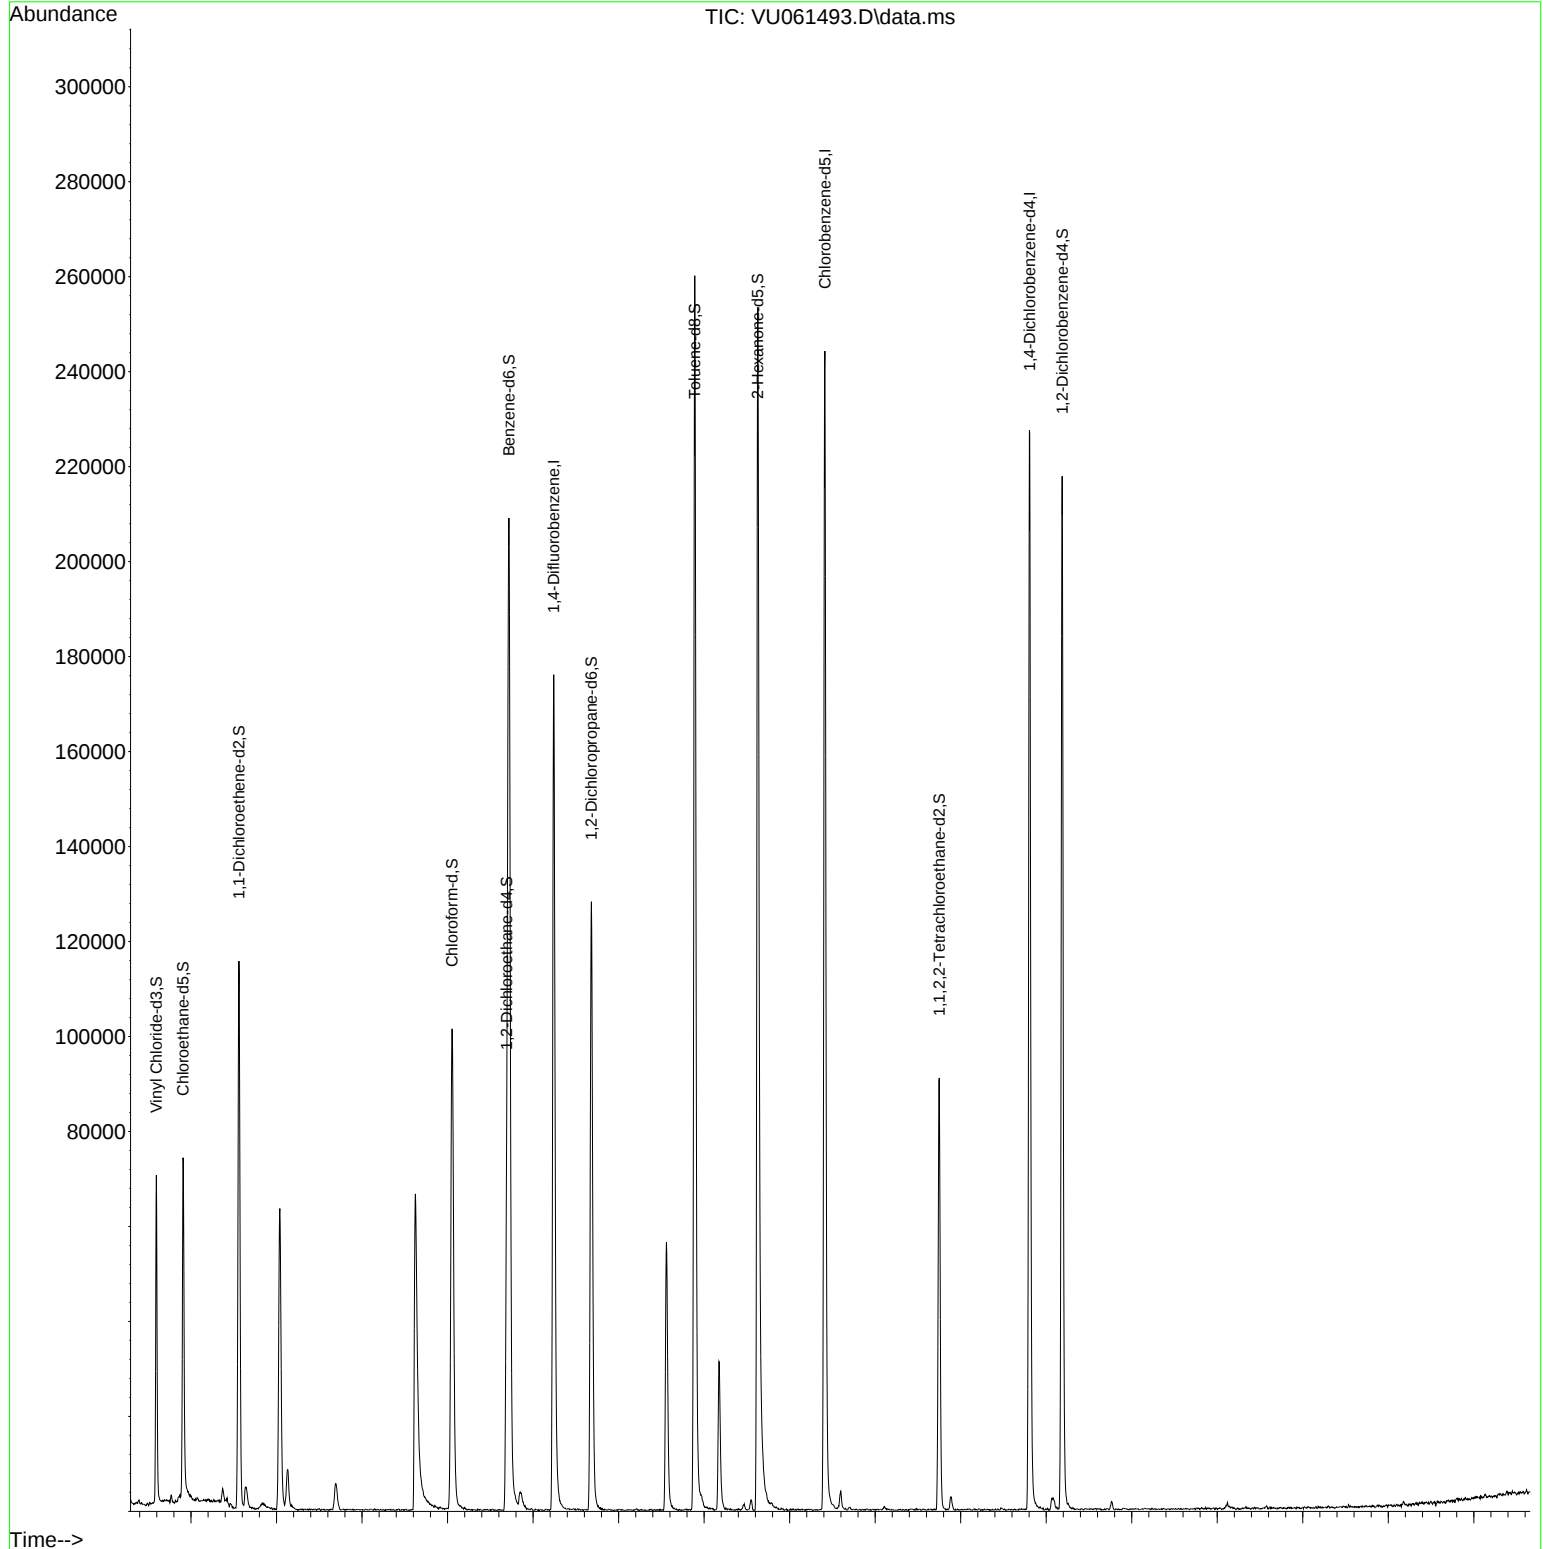

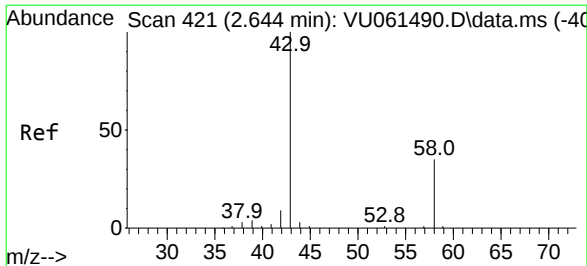

#13

Acetone

Concen: 5.025 ug/L

RT: 2.644 min Scan# 421

Delta R.T. -0.000 min

Lab File: VU061493.D

Acq: 06 Nov 2024 11:38

Instrument :

MSVOA_U

ClientSampleId :





C0AJ9

Tgt Ion: 43 Resp: 6663

Ion Ratio Lower Upper

43 100

58 30.6 0.0 73.2

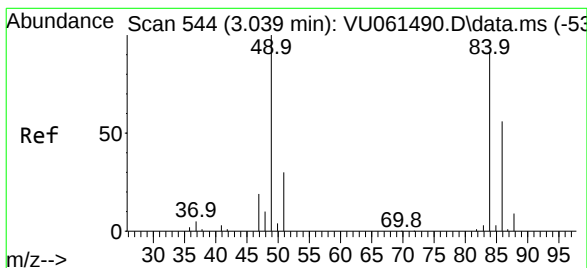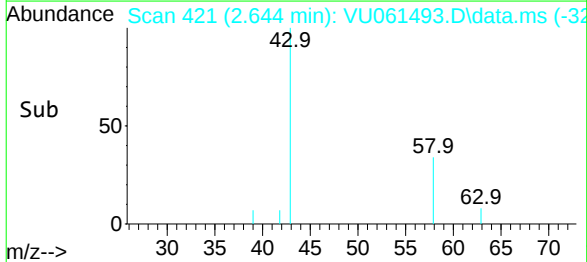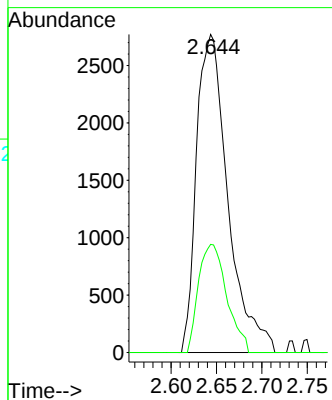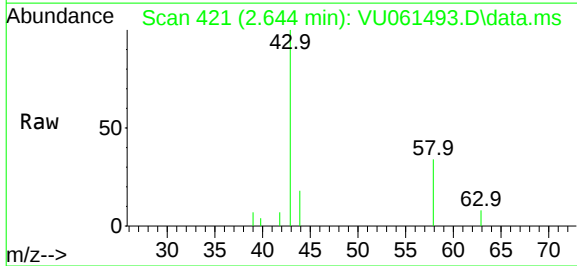

#16

Methylene chloride

Concen: 3.181 ug/L

RT: 3.039 min Scan# 544

Delta R.T. -0.000 min

Lab File: VU061493.D

Acq: 06 Nov 2024 11:38

Tgt Ion: 84 Resp: 33646

Ion Ratio Lower Upper

84 100

86 64.5 43.5 80.7

49 113.1 75.7 140.7

