

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
 Data File : VU061501.D
 Acq On : 06 Nov 2024 14:54
 Operator : MD/SY
 Sample : P4689-13DL 100X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CD9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rBV	65472	74463	13.86%	1.655%
2	1.911	184	193	207	rBV	66821	91216	16.97%	2.028%
3	2.560	384	395	417	rBV	111524	182507	33.96%	4.057%
4	3.181	573	588	603	rBV	13615	31104	5.79%	0.691%
5	3.695	736	748	759	rBV4	4654	10841	2.02%	0.241%
6	4.627	1022	1038	1081	rBV	76882	222773	41.46%	4.952%
7	5.052	1155	1170	1199	rBV2	100601	229134	42.64%	5.094%
8	5.717	1358	1377	1399	rBV2	208582	537356	100.00%	11.946%
9	6.242	1528	1540	1567	rBV	134108	267731	49.82%	5.952%
10	6.682	1664	1677	1702	rBV	123754	250317	46.58%	5.565%
11	7.560	1939	1950	1974	rBV	56315	103736	19.30%	2.306%
12	7.891	2040	2053	2082	rBV	252082	449732	83.69%	9.998%
13	8.174	2131	2141	2161	rBV	30726	55792	10.38%	1.240%
14	8.547	2245	2257	2272	rBV	200944	347023	64.58%	7.714%
15	8.627	2272	2282	2323	rVB2	252646	508350	94.60%	11.301%
16	9.412	2514	2526	2554	rBV	192793	339256	63.13%	7.542%
17	10.746	2930	2941	2957	rBV	92120	151309	28.16%	3.364%
18	11.804	3258	3270	3292	rBV	174936	292252	54.39%	6.497%
19	12.187	3374	3389	3408	rBV	210152	353445	65.77%	7.857%




Sum of corrected areas: 4498337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061501.D
Acq On : 06 Nov 2024 14:54
Operator : MD/SY
Sample : P4689-13DL 100X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

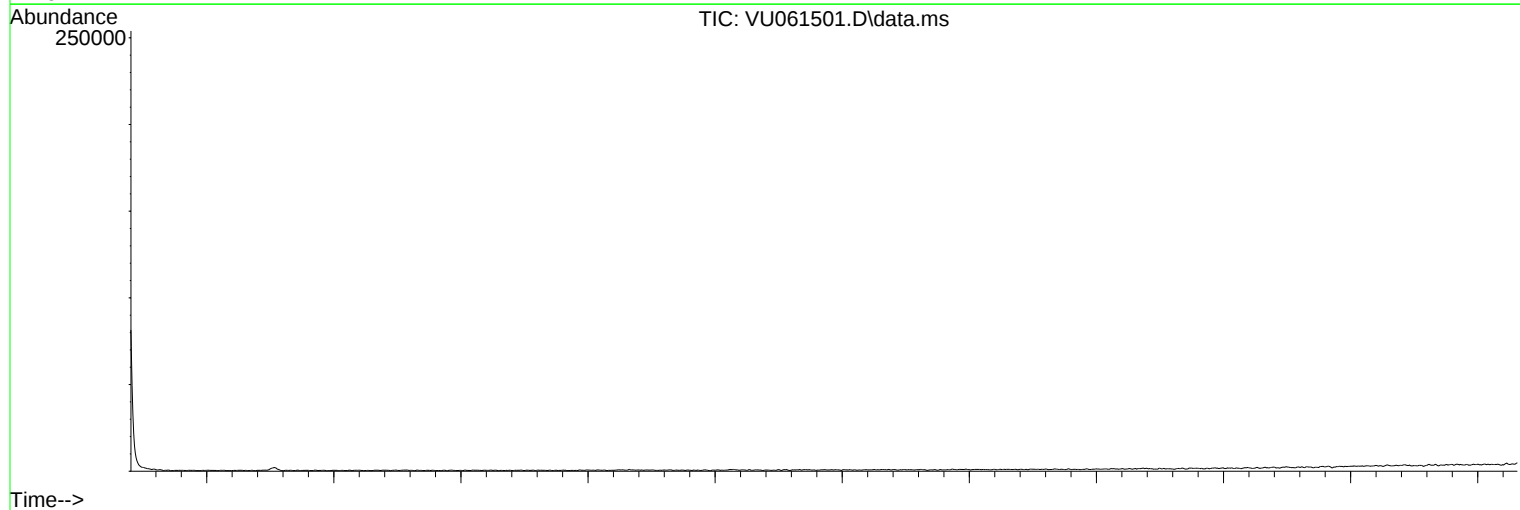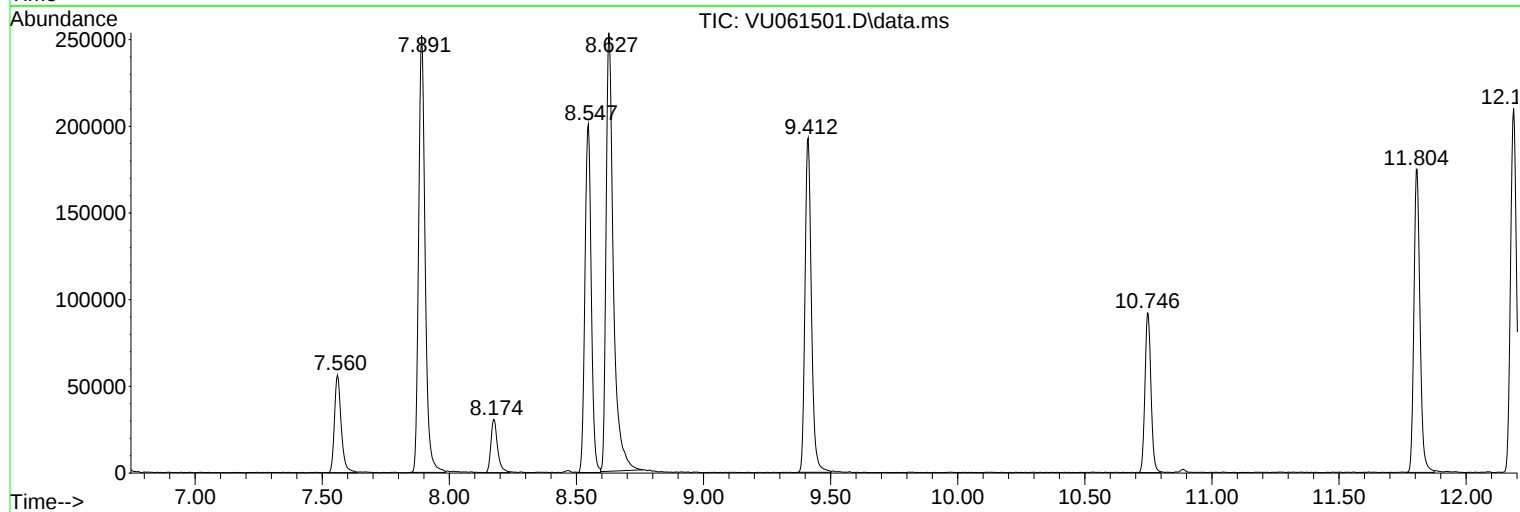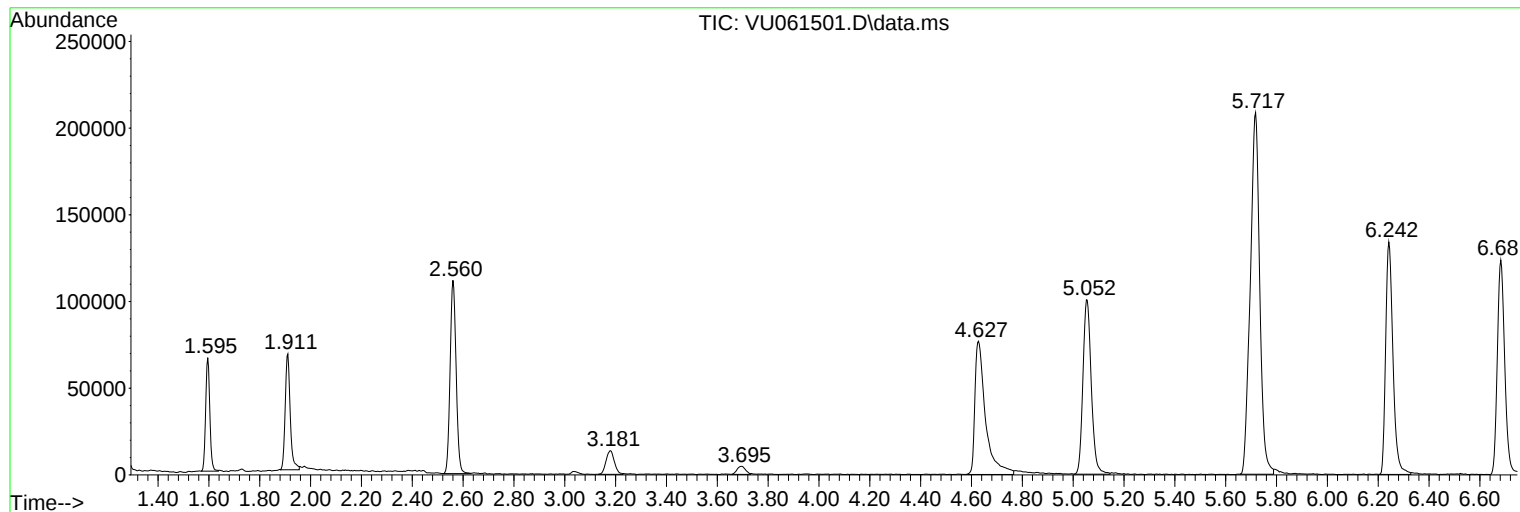

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061501.D
Acq On : 06 Nov 2024 14:54
Operator : MD/SY
Sample : P4689-13DL 100X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061501.D
Acq On : 06 Nov 2024 14:54
Operator : MD/SY
Sample : P4689-13DL 100X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
