

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
 Data File : VU061508.D
 Acq On : 06 Nov 2024 17:46
 Operator : MD/SY
 Sample : VIBLK158
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK158

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	105	rBV	58924	62943	11.74%	1.325%
2	1.907	184	192	205	rBV	61503	85554	15.96%	1.801%
3	2.560	382	395	415	rVB	98731	159126	29.68%	3.350%
4	3.181	573	588	606	rVB2	6714	15945	2.97%	0.336%
5	3.695	735	748	761	rBV4	6220	14802	2.76%	0.312%
6	4.628	1024	1038	1070	rBV	74348	205800	38.39%	4.332%
7	5.055	1156	1171	1196	rBV	96233	220611	41.15%	4.644%
8	5.718	1358	1377	1402	rBV2	199604	520724	97.13%	10.962%
9	6.242	1527	1540	1570	rBV	186880	364679	68.02%	7.677%
10	6.682	1664	1677	1701	rBV	122745	245360	45.77%	5.165%
11	7.560	1936	1950	1977	rBV	53046	100592	18.76%	2.118%
12	7.891	2040	2053	2077	rBV	240381	427277	79.70%	8.995%
13	8.174	2130	2141	2158	rBV2	29921	53815	10.04%	1.133%
14	8.627	2271	2282	2317	rBV	264947	536127	100.00%	11.286%
15	9.412	2513	2526	2550	rBV	261191	454592	84.79%	9.570%
16	10.746	2926	2941	2958	rBV	91537	152103	28.37%	3.202%
17	11.804	3259	3270	3291	rBV	244944	408113	76.12%	8.591%
18	12.087	3346	3358	3371	rBV	27233	40949	7.64%	0.862%
19	12.187	3377	3389	3409	rBV	209858	353070	65.86%	7.432%
20	12.930	3610	3620	3628	rBV2	3843	5951	1.11%	0.125%
21	13.032	3642	3652	3667	rBV5	6406	14422	2.69%	0.304%
22	13.450	3773	3782	3791	rBV3	6366	8654	1.61%	0.182%
23	14.081	3965	3978	4001	rBV	127145	224287	41.83%	4.721%
24	14.206	4007	4017	4030	rBV	19954	33365	6.22%	0.702%
25	15.225	4325	4334	4351	rVV3	6361	12443	2.32%	0.262%
26	15.409	4381	4391	4404	rBV	15933	29116	5.43%	0.613%

Sum of corrected areas: 4750420




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061508.D
Acq On : 06 Nov 2024 17:46
Operator : MD/SY
Sample : VIBLK158
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

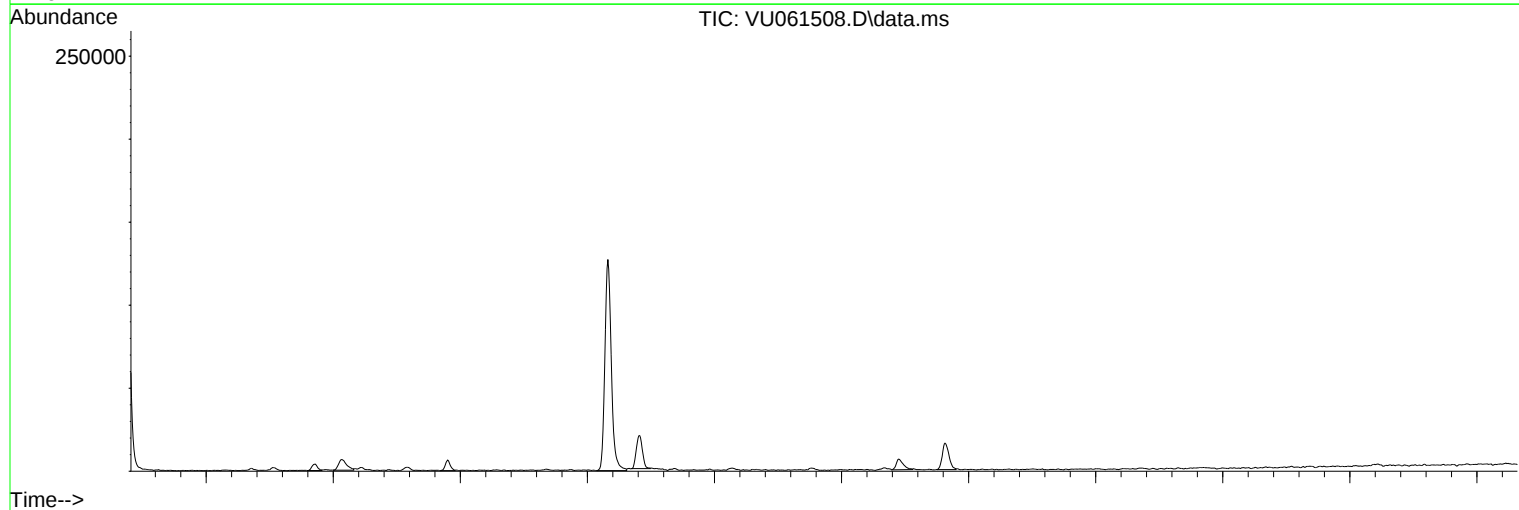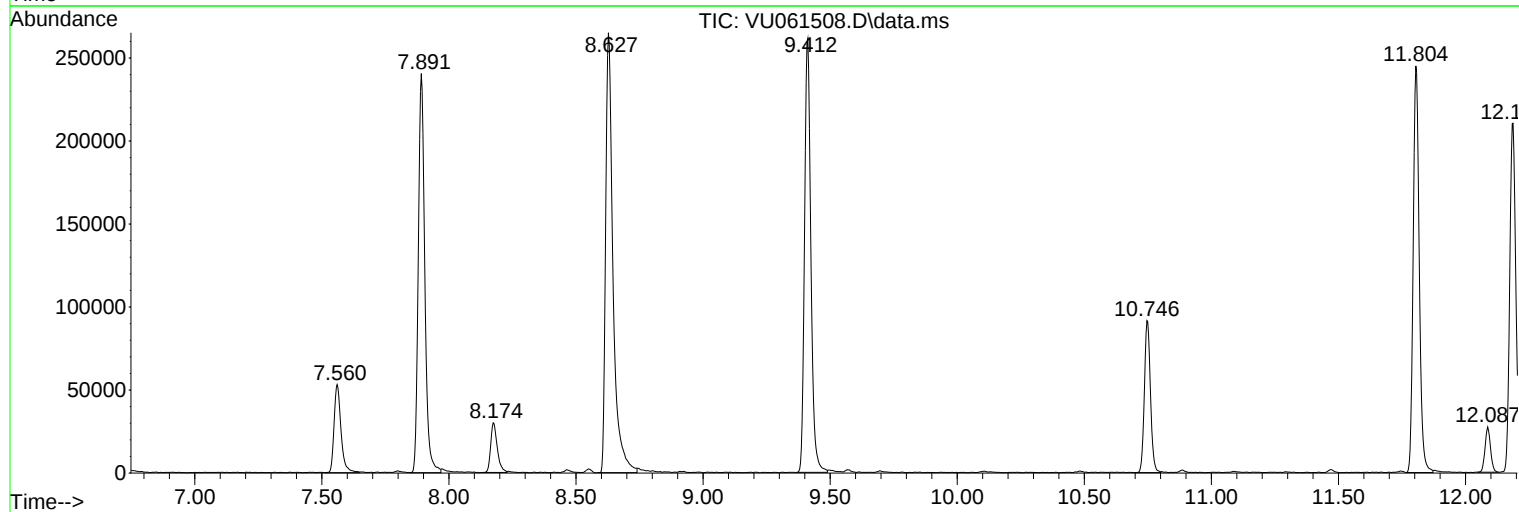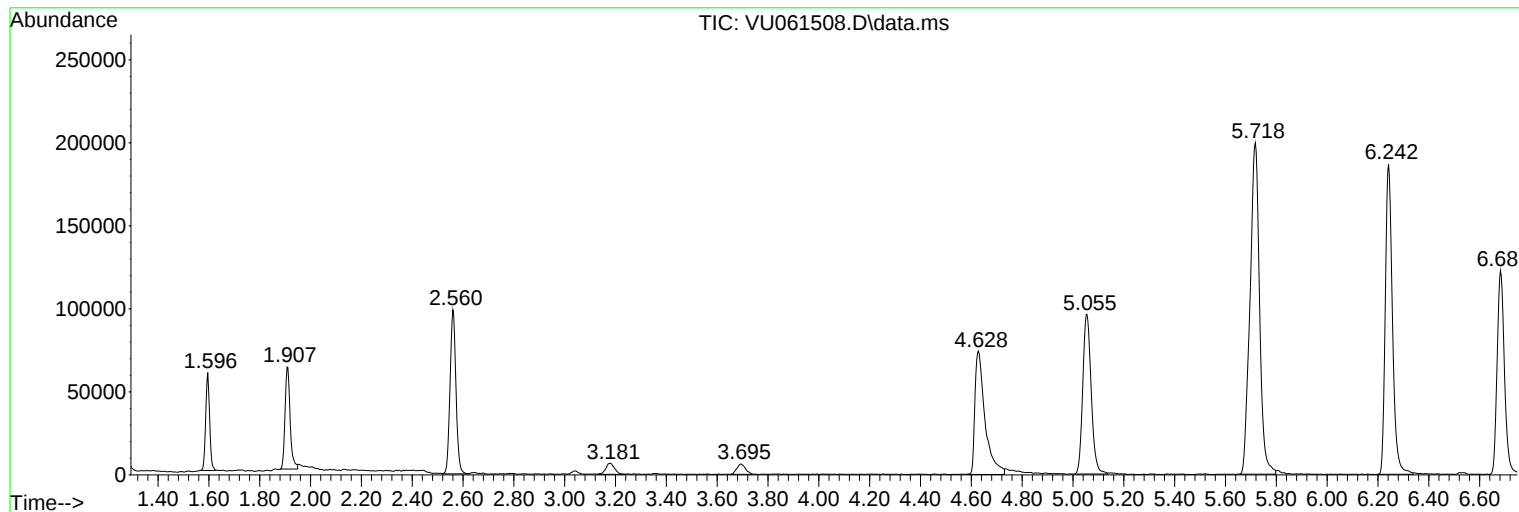

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061508.D
Acq On : 06 Nov 2024 17:46
Operator : MD/SY
Sample : VIBLK158
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061508.D
Acq On : 06 Nov 2024 17:46
Operator : MD/SY
Sample : VIBLK158
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc