

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
 Data File : VU061511.D
 Acq On : 06 Nov 2024 19:00
 Operator : MD/SY
 Sample : P4714-10
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAH0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	80	95	111	rBV	66833	81641	15.26%	1.865%
2	1.727	129	136	146	rVB	17498	21022	3.93%	0.480%
3	1.907	183	192	209	rVB	71194	95720	17.89%	2.187%
4	2.560	378	395	413	rBV	110317	180350	33.71%	4.120%
5	3.692	736	747	762	rBV5	5362	12397	2.32%	0.283%
6	4.621	1027	1036	1071	rBV	66877	178755	33.41%	4.084%
7	5.055	1156	1171	1190	rBV	97480	218298	40.80%	4.987%
8	5.718	1358	1377	1410	rBV2	204901	535000	100.00%	12.222%
9	6.242	1526	1540	1562	rBV	166080	325180	60.78%	7.429%
10	6.682	1663	1677	1702	rBV2	121515	245869	45.96%	5.617%
11	7.560	1939	1950	1970	rBV	54726	100686	18.82%	2.300%
12	7.891	2039	2053	2068	rBV	248676	442959	82.80%	10.120%
13	7.965	2068	2076	2097	rVB	25853	49181	9.19%	1.124%
14	8.174	2128	2141	2161	rBV3	29124	54000	10.09%	1.234%
15	8.627	2271	2282	2320	rBV2	258614	514724	96.21%	11.759%
16	9.409	2514	2525	2557	rBV	233943	414174	77.42%	9.462%
17	10.746	2928	2941	2965	rBV	93329	152832	28.57%	3.492%
18	11.804	3255	3270	3294	rBV	219088	365522	68.32%	8.351%
19	12.087	3349	3358	3370	rVB3	8743	13567	2.54%	0.310%
20	12.187	3377	3389	3417	rBV	210683	359822	67.26%	8.220%
21	14.093	3972	3982	3997	rBV2	8273	15503	2.90%	0.354%




Sum of corrected areas: 4377202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061511.D
Acq On : 06 Nov 2024 19:00
Operator : MD/SY
Sample : P4714-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

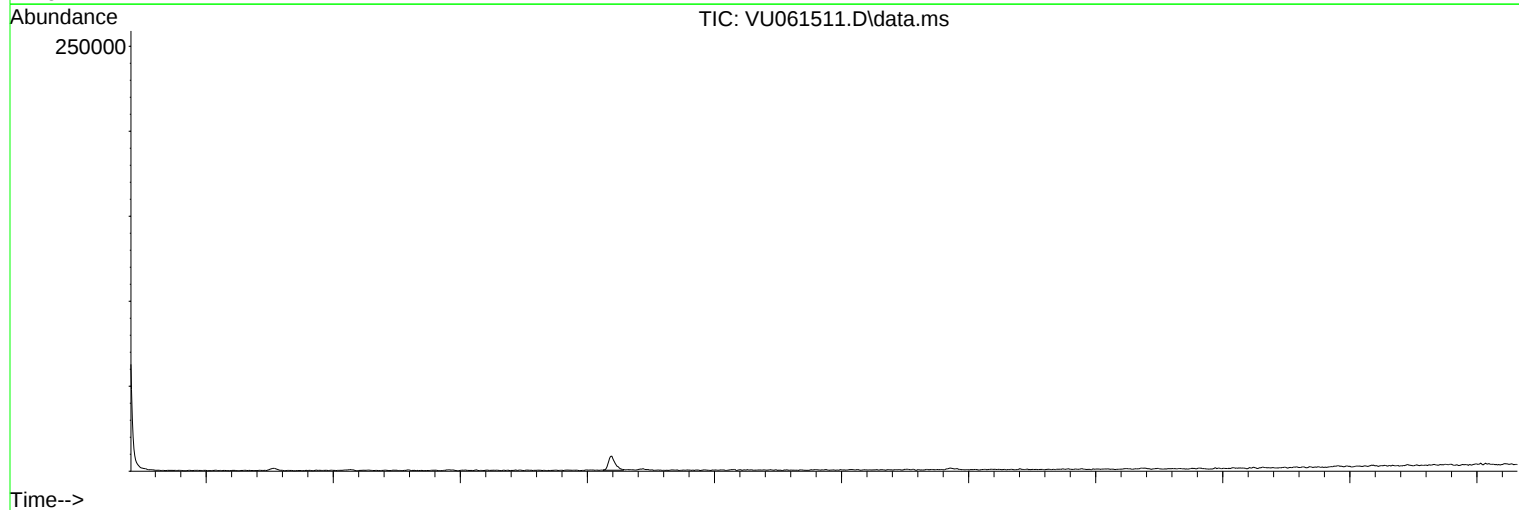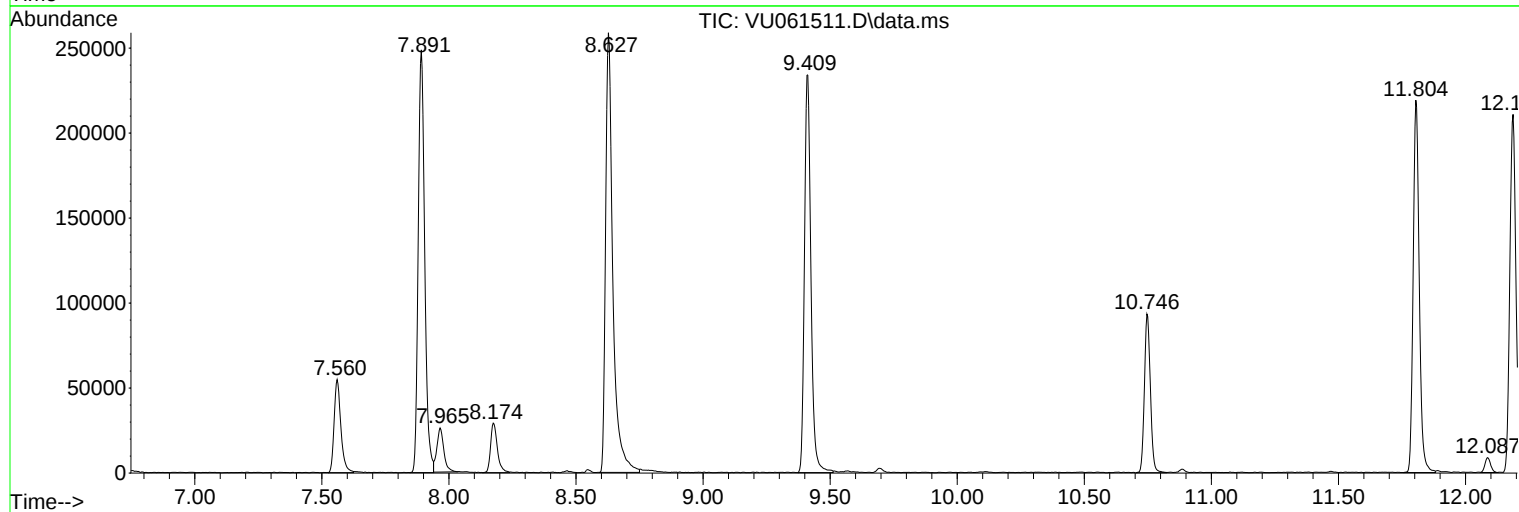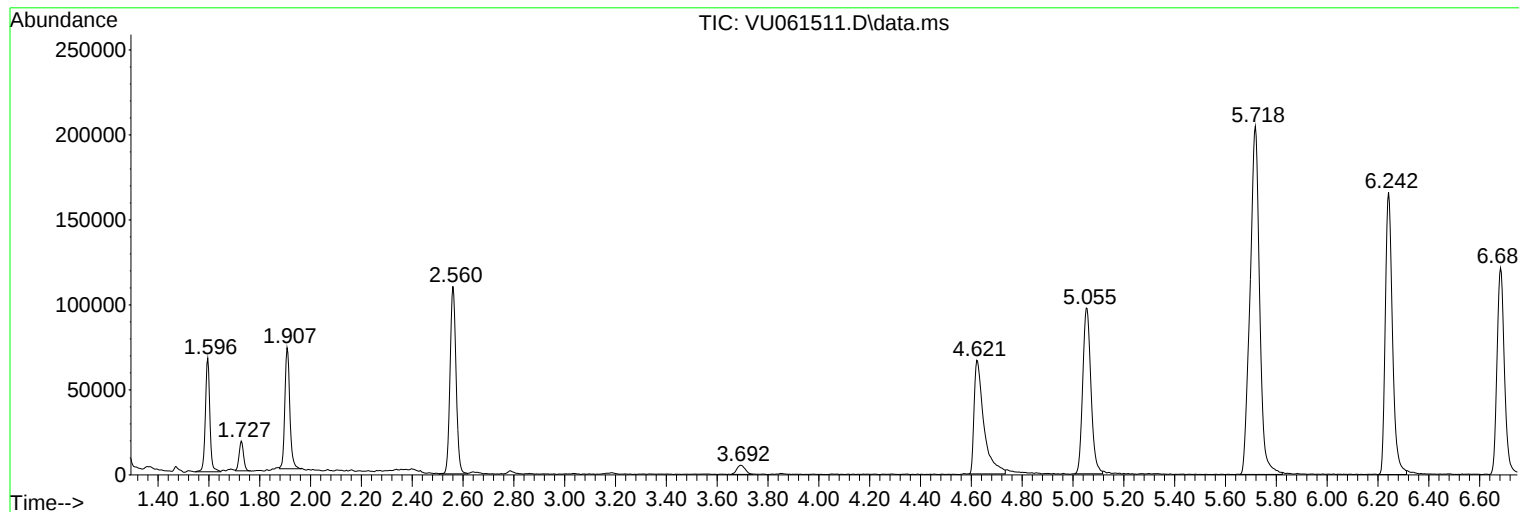

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061511.D
Acq On : 06 Nov 2024 19:00
Operator : MD/SY
Sample : P4714-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061511.D
Acq On : 06 Nov 2024 19:00
Operator : MD/SY
Sample : P4714-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------