


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110624\
Data File : VU061489.D
Acq On : 06 Nov 2024 09:13
Operator : MD/SY
Sample : BFB021
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB021

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 07 00:10:32 2024

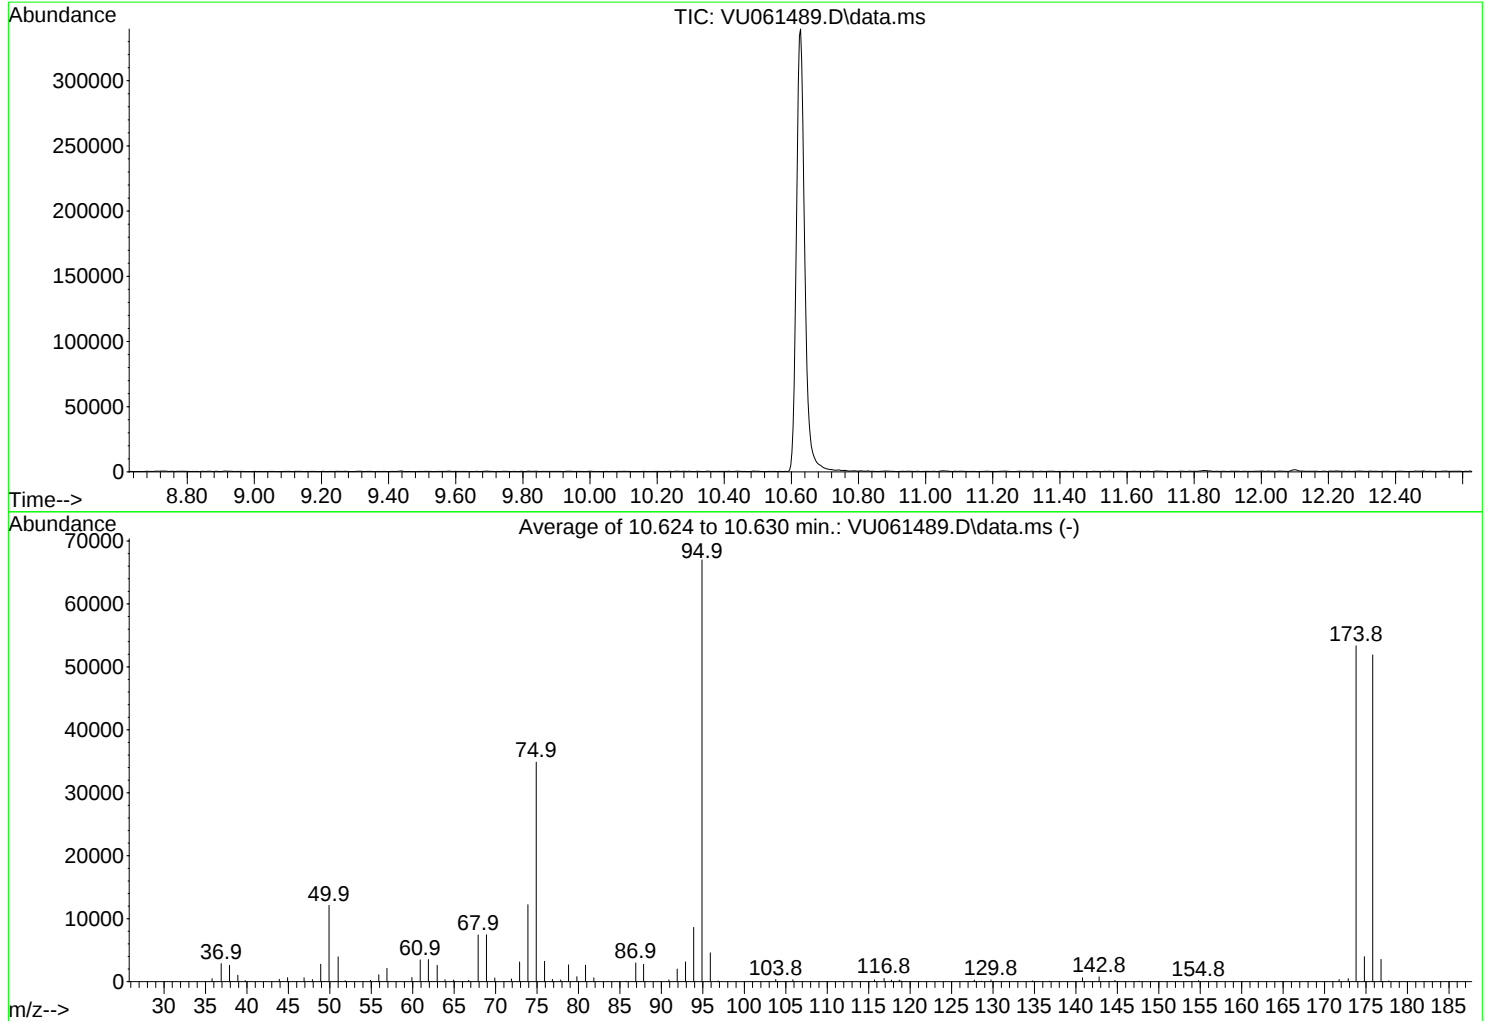

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	12117	PASS
75	95	30	80	52.1	34877	PASS
95	95	100	100	100.0	67005	PASS
96	95	5	9	6.8	4579	PASS
173	174	0.00	2	0.9	489	PASS
174	95	50	120	79.6	53347	PASS
175	174	5	9	7.5	3976	PASS
176	174	95	101	97.3	51915	PASS
177	176	5	9	6.8	3537	PASS

m/z	Abundance
43.90	372.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.80	513.0
36.90	3003.0
37.90	2729.0
38.90	1077.0
39.80	162.0
43.90	725.0
44.90	654.0
46.90	722.0
47.90	354.0
48.90	2900.0
49.90	12596.0
51.00	3948.0
51.80	195.0
54.90	205.0
55.90	1218.0
56.90	2187.0
59.90	688.0
60.90	3642.0
61.90	3635.0
63.00	2670.0
63.90	322.0
64.90	272.0
66.80	181.0
67.90	7417.0
68.90	7762.0
69.90	625.0
71.90	412.0
72.90	3167.0
73.90	12476.0
74.90	35072.0
75.90	3355.0
76.90	381.0
77.80	247.0
78.80	2683.0
79.80	883.0
80.80	2515.0
81.90	591.0
86.90	3127.0
87.80	2894.0
90.90	249.0
91.90	1936.0
92.90	3094.0
93.90	8632.0
94.90	68248.0
95.90	4729.0
96.90	110.0
103.80	349.0
105.90	309.0
115.70	277.0
116.90	500.0
117.80	206.0
118.70	383.0
127.70	233.0
128.60	122.0
129.70	247.0
134.80	122.0
136.80	145.0
140.80	624.0
142.80	740.0
144.70	230.0
147.70	115.0
154.80	178.0
156.80	112.0
171.80	363.0
172.90	563.0
173.80	53576.0
174.80	4030.0
175.80	51984.0
176.80	3619.0
177.70	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.80	495.0
36.90	2925.0
37.90	2662.0
38.90	1032.0
39.80	162.0
43.90	770.0
44.90	642.0
46.90	634.0
47.90	340.0
48.90	2890.0
49.90	12475.0
51.00	4073.0
51.90	151.0
54.90	195.0
55.90	1097.0
56.90	2170.0
59.90	691.0
60.90	3598.0
61.90	3654.0
62.90	2683.0
63.90	298.0
64.90	267.0
66.80	211.0
67.90	7720.0
68.90	7648.0
69.90	614.0
71.90	447.0
72.90	3209.0
73.90	12614.0
74.90	35808.0
75.90	3350.0
76.80	354.0
77.80	293.0
78.80	2761.0
79.80	805.0
80.90	2704.0
81.80	626.0
85.80	122.0
86.90	3015.0
87.90	2783.0
90.90	278.0
91.90	2097.0
92.90	3236.0
93.90	8874.0
94.90	69072.0
95.90	4772.0
96.80	117.0
103.80	361.0
105.80	323.0
115.70	292.0
116.80	535.0
117.70	263.0
118.70	370.0
127.80	261.0
128.60	107.0
129.80	283.0
134.70	127.0
136.80	115.0
140.80	651.0
142.80	806.0
144.70	235.0
147.60	107.0
154.80	190.0
171.80	386.0
172.90	499.0
173.80	54968.0
174.80	4088.0
175.80	53496.0
176.80	3610.0
177.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.80	430.0
36.90	2684.0
37.90	2420.0
38.90	933.0
39.80	194.0
43.90	745.0
44.90	581.0
46.90	501.0
47.90	307.0
48.90	2556.0
49.90	11281.0
51.00	3821.0
51.90	120.0
54.90	182.0
55.90	981.0
56.90	1969.0
59.90	628.0
60.90	3172.0
61.90	3249.0
62.90	2461.0
63.90	302.0
65.00	263.0
66.70	187.0
67.90	7108.0
68.90	6936.0
69.90	531.0
71.90	439.0
72.90	3016.0
73.90	11624.0
74.90	33752.0
75.90	2993.0
76.80	332.0
77.90	301.0
78.80	2542.0
79.80	683.0
80.90	2629.0
81.80	622.0
85.70	139.0
86.90	2756.0
87.90	2586.0
90.90	282.0
91.90	1966.0
92.90	3033.0
93.90	8333.0
94.90	63696.0
95.90	4235.0
96.90	109.0
103.80	352.0
104.90	106.0
105.80	293.0
115.70	302.0
116.80	502.0
117.70	306.0
118.90	352.0
127.80	250.0
129.80	296.0
134.70	121.0
140.80	589.0
141.80	116.0
142.80	760.0
144.70	183.0
145.80	100.0
154.80	189.0
171.70	349.0
172.80	406.0
173.80	51496.0
174.80	3810.0
175.80	50264.0
176.80	3381.0
177.80	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021