

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110724\
 Data File : VU061520.D
 Acq On : 07 Nov 2024 14:41
 Operator : MD/SY
 Sample : P4743-01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H46Q8

Quant Time: Nov 08 00:28:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 08 00:26:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	143513	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	136132	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	60182	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	45047	4.621	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.907	69	49935	5.587	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.800%
11) 1,1-Dichloroethene-d2	2.560	65	22082	5.294	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.800%
20) 2-Butanone-d5	4.624	46	108362	54.747	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.500%
24) Chloroform-d	5.055	84	98572	5.327	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.600%
26) 1,2-Dichloroethane-d4	5.695	65	50235	5.446	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.000%
32) Benzene-d6	5.721	84	198414	5.173	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	6.682	67	61770	5.356	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%
41) Toluene-d8	7.891	98	177530	4.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	8.177	79	19687	4.182	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.627	63	89112	46.219	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.440%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	45640	5.233	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	58047	5.447	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.000%
Target Compounds					Qvalue	
13) Acetone	2.640	43	5644	4.502	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110724\
Data File : VU061520.D
Acq On : 07 Nov 2024 14:41
Operator : MD/SY
Sample : P4743-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46Q8


Quant Time: Nov 08 00:28:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 08 00:26:16 2024
Response via : Initial Calibration

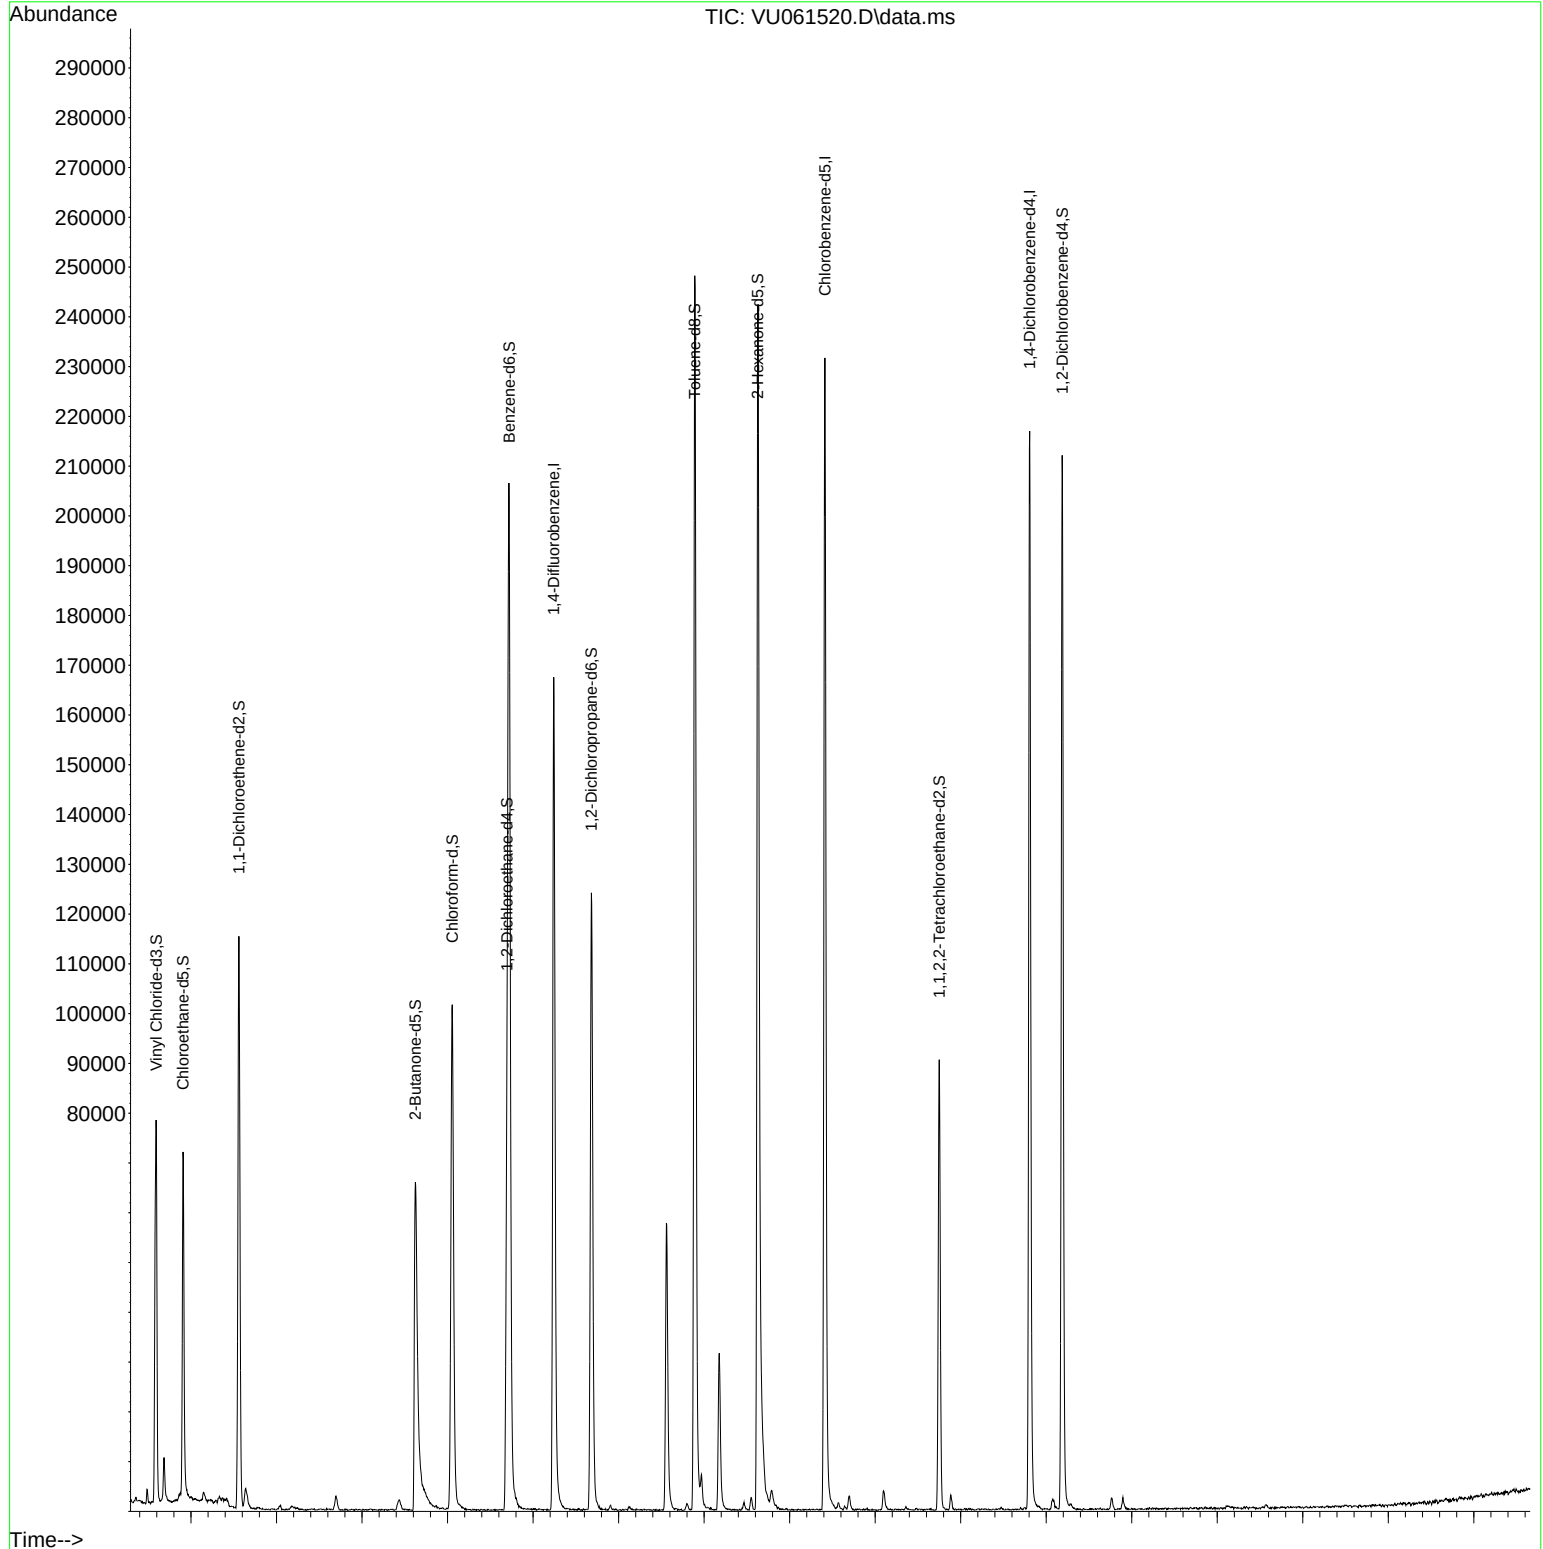

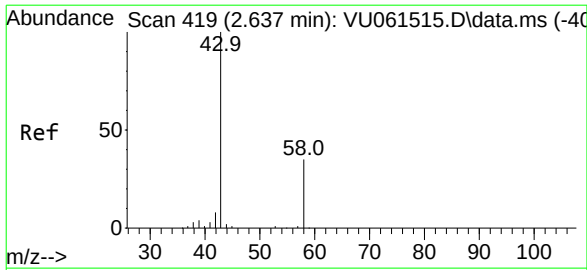

#13
Acetone
Concen: 4.502 ug/L
RT: 2.640 min Scan# 42
Delta R.T. 0.003 min
Lab File: VU061520.D
Acq: 07 Nov 2024 14:41

Instrument :
MSVOA_U
ClientSampleId :
H46Q8

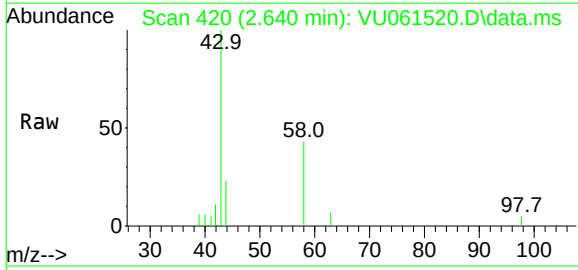

Tgt Ion: 43 Resp: 5644
Ion Ratio Lower Upper
43 100
58 34.9 0.0 73.2

