
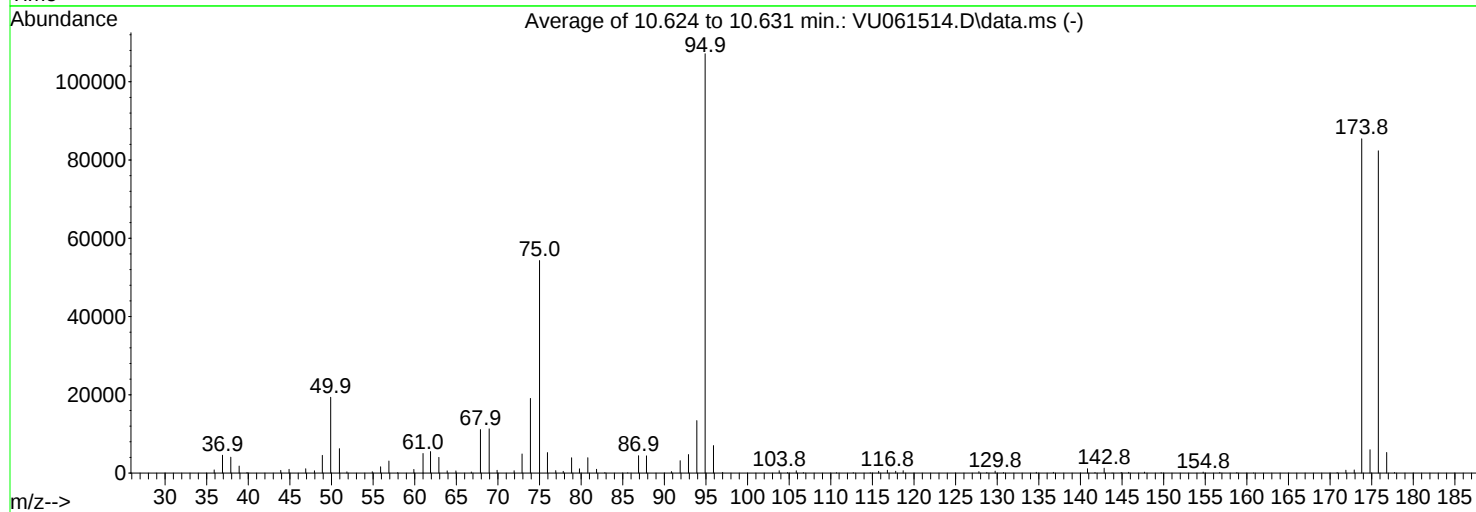


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110724\
Data File : VU061514.D
Acq On : 07 Nov 2024 09:37
Operator : MD/SY
Sample : BFB022
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 08 00:26:16 2024

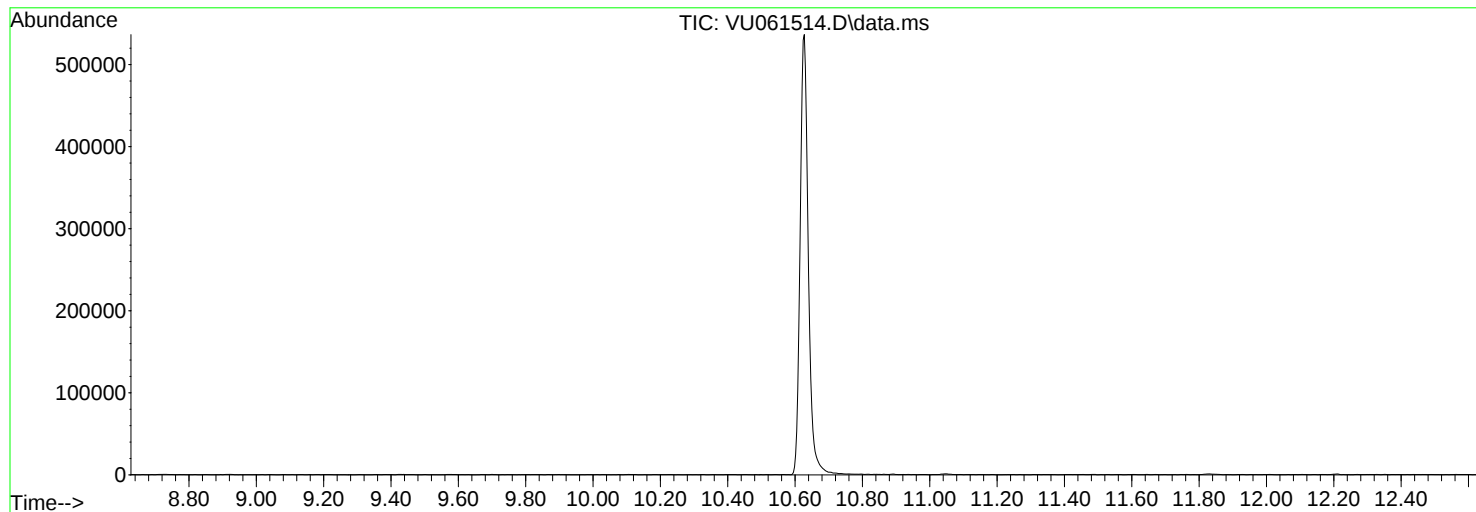

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	19371	PASS
75	95	30	80	50.7	54315	PASS
95	95	100	100	100.0	107160	PASS
96	95	5	9	6.6	7025	PASS
173	174	0.00	2	0.9	798	PASS
174	95	50	120	79.7	85416	PASS
175	174	5	9	7.0	5958	PASS
176	174	95	101	96.4	82352	PASS
177	176	5	9	6.4	5265	PASS

m/z	Abundance
43.90	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	900.0
36.90	4770.0
37.90	4105.0
38.90	1882.0
39.80	168.0
43.90	1040.0
44.90	1000.0
46.90	1072.0
48.00	527.0
48.90	4829.0
49.90	20272.0
50.90	6549.0
51.90	362.0
54.90	342.0
55.90	1681.0
56.90	3141.0
58.00	163.0
59.90	890.0
61.00	5228.0
61.90	5698.0
62.90	4247.0
63.90	587.0
64.90	586.0
66.70	285.0
67.90	11506.0
68.90	11560.0
69.90	757.0
72.00	662.0
72.90	5238.0
73.90	19816.0
75.00	55856.0
75.90	5337.0
76.90	681.0
77.80	461.0
78.90	4081.0
79.80	1146.0
80.80	4159.0
81.80	998.0
82.90	106.0
85.60	147.0
86.90	4658.0
87.90	4294.0
90.90	311.0
91.90	3235.0
92.90	4934.0
93.90	13943.0
94.90	108848.0
95.90	7228.0
97.00	153.0
103.80	592.0
104.80	143.0
105.80	555.0
106.70	127.0
110.70	111.0
112.70	139.0
115.80	424.0
116.80	731.0
117.80	574.0
118.70	606.0
127.80	371.0
128.80	147.0
129.70	482.0
130.80	143.0
134.70	159.0
136.70	171.0
140.90	1171.0
141.80	134.0
142.90	1251.0
143.80	115.0
144.90	203.0
145.80	230.0
147.70	213.0
149.80	119.0
154.80	267.0
156.70	192.0
158.80	149.0
170.90	131.0
171.90	714.0
172.90	779.0
173.80	85048.0
174.80	5919.0
175.80	81888.0
176.80	5236.0
177.80	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	824.0
36.90	4694.0
37.90	4211.0
38.90	1850.0
39.90	165.0
43.90	1018.0
44.90	1001.0
46.90	1166.0
48.00	599.0
48.90	4660.0
49.90	19912.0
50.90	6493.0
51.90	340.0
54.90	350.0
55.90	1634.0
56.90	3184.0
57.90	136.0
59.90	967.0
61.00	5191.0
61.90	5595.0
62.90	4095.0
63.90	578.0
65.00	584.0
66.80	280.0
67.90	11399.0
68.90	11624.0
69.90	722.0
72.00	627.0
72.90	5013.0
73.90	19552.0
75.00	55816.0
76.00	5425.0
76.90	599.0
77.90	486.0
78.80	3968.0
79.80	1100.0
80.80	3985.0
81.90	1005.0
82.80	127.0
85.60	104.0
86.90	4463.0
87.80	4443.0
90.80	379.0
91.90	3265.0
92.90	4836.0
93.90	13812.0
94.90	110616.0
95.90	7227.0
97.00	169.0
103.80	642.0
104.80	123.0
105.90	605.0
106.70	141.0
110.70	113.0
112.70	133.0
114.70	111.0
115.80	479.0
116.80	759.0
117.80	468.0
118.70	649.0
127.80	398.0
128.70	193.0
129.80	536.0
130.70	138.0
134.70	200.0
136.70	199.0
140.80	1164.0
141.80	158.0
142.80	1253.0
144.90	167.0
145.80	192.0
147.70	248.0
149.70	123.0
154.80	261.0
156.70	197.0
158.80	161.0
170.90	166.0
171.90	771.0
172.90	809.0
173.80	87968.0
174.80	6157.0
175.80	84992.0
176.80	5391.0
177.80	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	704.0
36.90	4243.0
37.90	3864.0
38.90	1643.0
39.80	146.0
43.90	977.0
44.90	864.0
46.90	1086.0
47.90	631.0
48.90	4101.0
49.90	17928.0
51.00	5700.0
51.80	258.0
54.90	357.0
55.90	1501.0
56.90	2915.0
59.90	945.0
61.00	4588.0
61.90	5184.0
62.90	3697.0
63.90	534.0
64.90	506.0
66.90	283.0
67.90	10431.0
69.00	10697.0
69.90	652.0
71.90	531.0
72.90	4392.0
73.90	17864.0
75.00	51272.0
76.00	4948.0
77.00	581.0
77.90	394.0
78.80	3697.0
79.80	1038.0
80.80	3650.0
81.80	899.0
82.80	142.0
86.90	4197.0
87.80	4464.0
90.80	446.0
91.90	3000.0
92.90	4446.0
93.90	12465.0
94.90	102016.0
95.90	6620.0
97.00	193.0
103.80	589.0
104.80	122.0
105.90	626.0
106.70	127.0
110.70	111.0
112.70	102.0
114.80	119.0
115.70	452.0
116.80	719.0
117.80	375.0
118.70	600.0
127.80	351.0
128.70	205.0
129.80	509.0
130.70	146.0
134.70	234.0
136.80	220.0
140.80	1030.0
141.70	142.0
142.80	1242.0
144.90	124.0
145.80	164.0
147.70	266.0
149.60	113.0
154.70	239.0
156.80	166.0
158.80	172.0
160.80	125.0
170.80	154.0
171.90	737.0
172.90	807.0
173.80	83232.0
174.80	5797.0
175.80	80176.0
176.80	5167.0
177.70	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022