

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
 Data File : VU045621.D
 Acq On : 08 Nov 2021 17:27
 Operator : SY/MD
 Sample : M4574-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TRIP-BLANK

Quant Time: Nov 09 09:59:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.375	168	151688	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	287177	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	289414	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	147893	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	123737	54.469	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	108.940%
35) Dibromofluoromethane	5.292	113	96910	50.544	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.080%
50) Toluene-d8	7.899	98	376083	52.750	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	105.500%
62) 4-Bromofluorobenzene	10.636	95	146744	51.328	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045621.D
Acq On : 08 Nov 2021 17:27
Operator : SY/MD
Sample : M4574-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK

Quant Time: Nov 09 09:59:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 05 13:35:16 2021
Response via : Initial Calibration




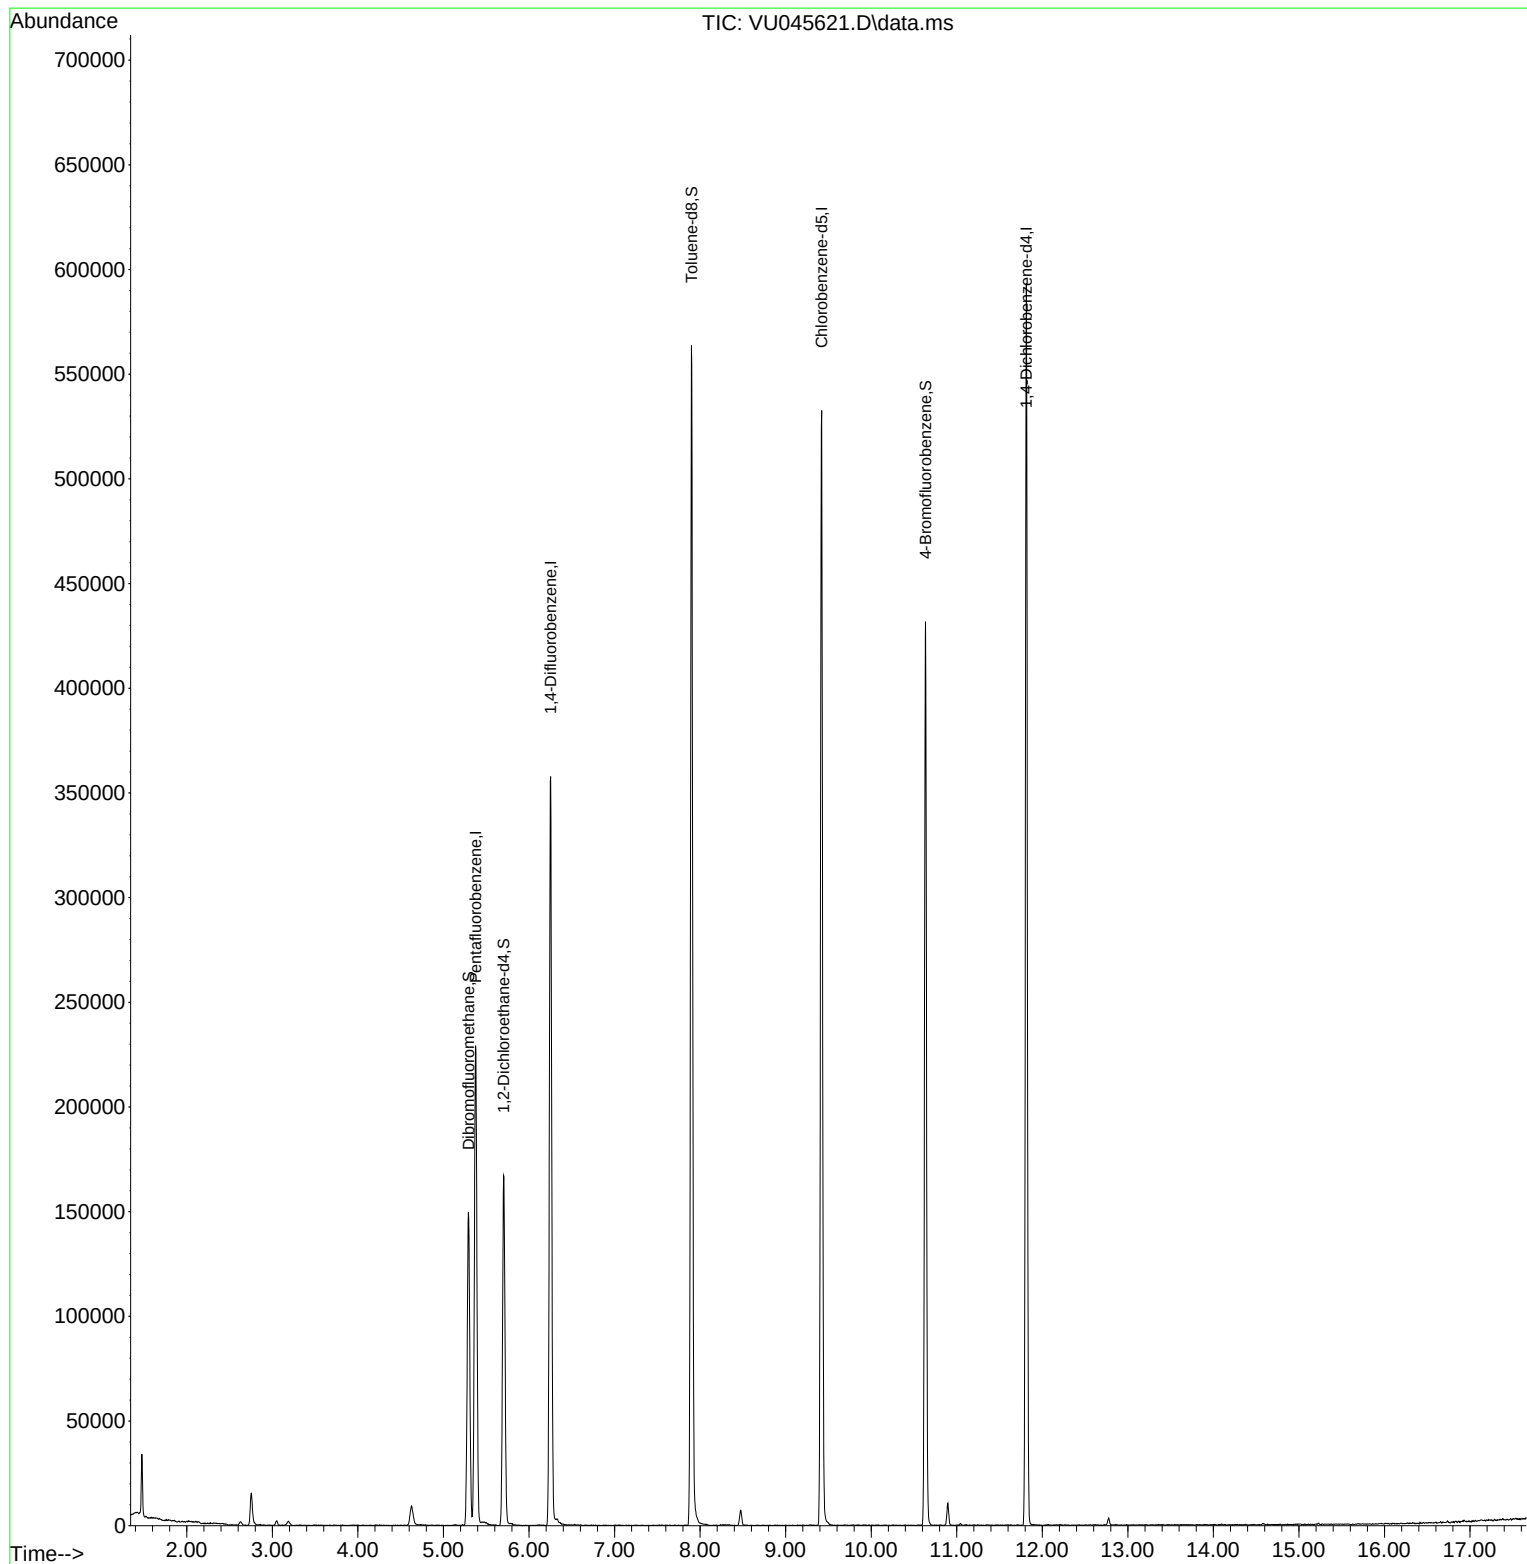


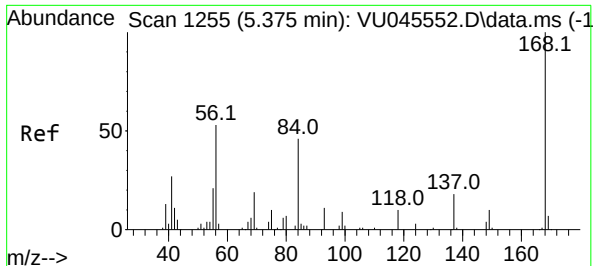

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. 0.000 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 151688
Ion Ratio Lower Upper
168 100
99 64.8 51.0 76.6

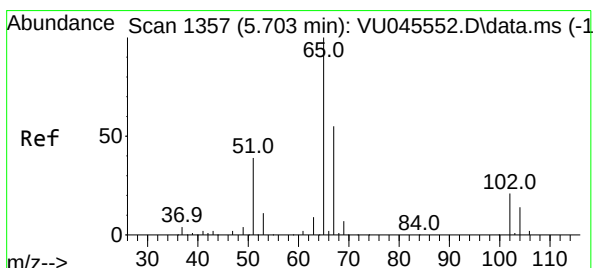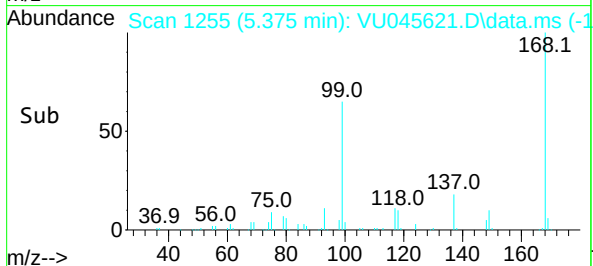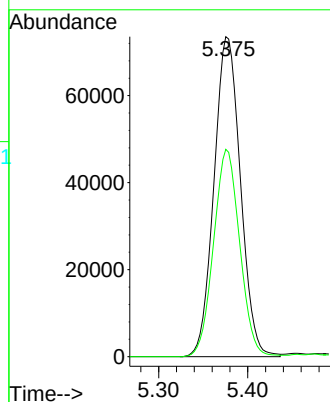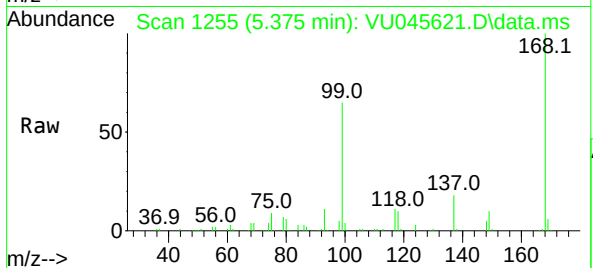

#33
1,2-Dichloroethane-d4
Concen: 54.469 ug/l
RT: 5.703 min Scan# 1357
Delta R.T. 0.000 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27

Tgt Ion: 65 Resp: 123737
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.8

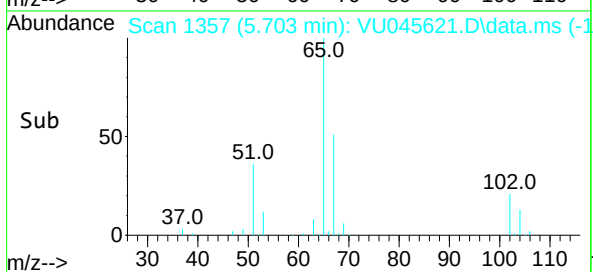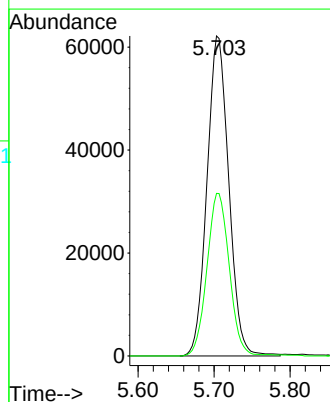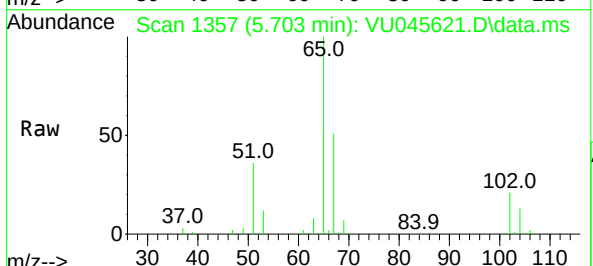

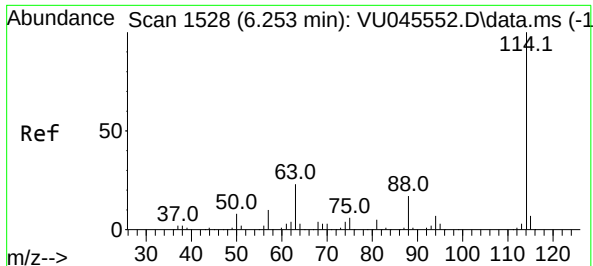

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 11

Delta R.T. 0.000 min

Lab File: VU045621.D

Acq: 08 Nov 2021 17:27

Instrument :

MSVOA_U

ClientSampleId :

TRIP-BLANK





Tgt Ion:114 Resp: 287177

Ion Ratio Lower Upper

114 100

63 21.9 0.0 45.6

88 16.7 0.0 33.8

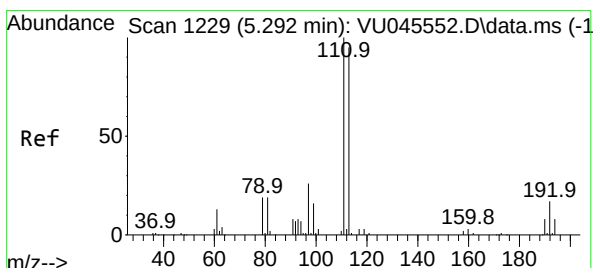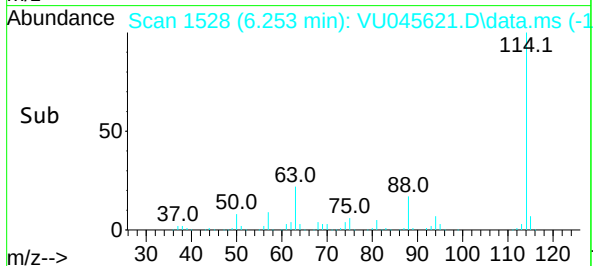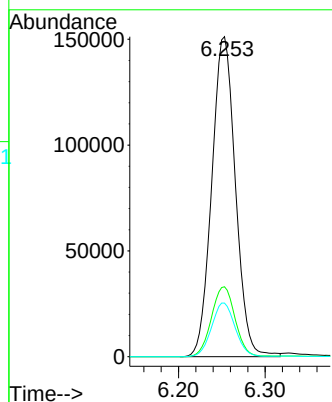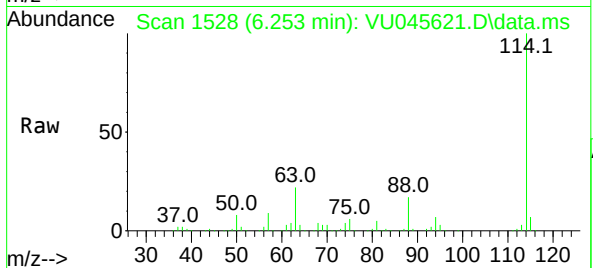

#35

Dibromofluoromethane

Concen: 50.544 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. 0.000 min

Lab File: VU045621.D

Acq: 08 Nov 2021 17:27




Tgt Ion:113 Resp: 96910


Ion Ratio Lower Upper

113 100

111 100.9 82.8 124.2

192 18.2 14.8 22.2


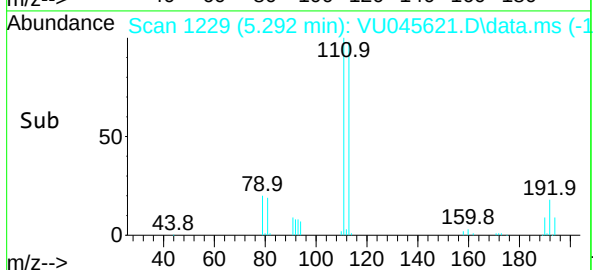
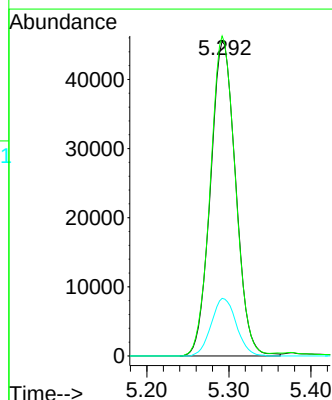
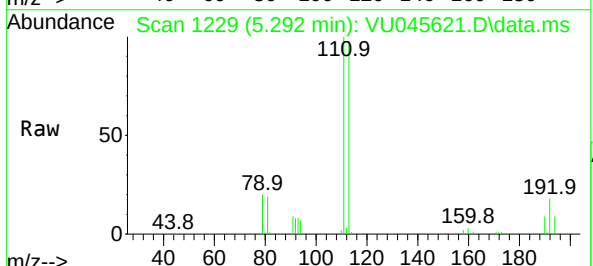


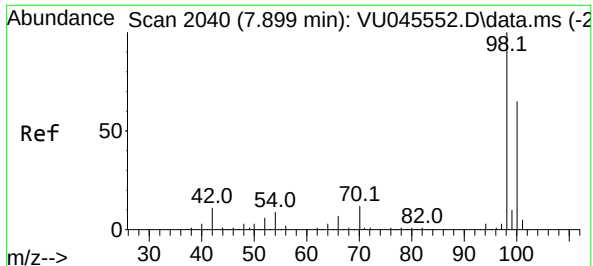

#50
Toluene-d8
Concen: 52.750 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. 0.000 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27




Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 376083
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

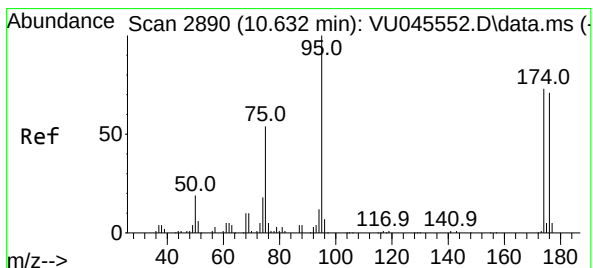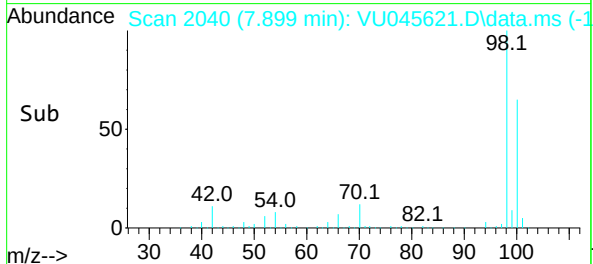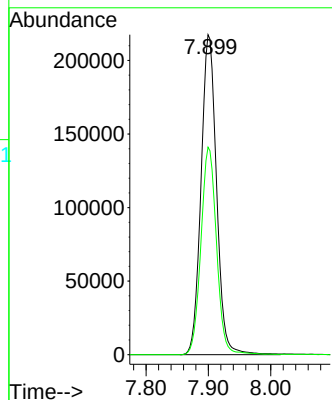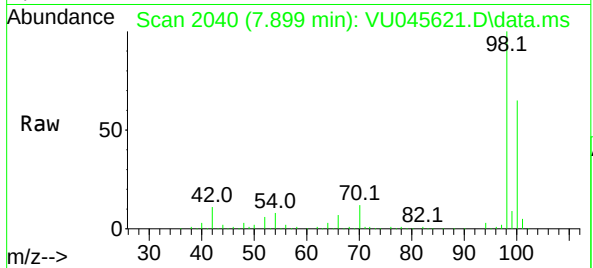

#62
4-Bromofluorobenzene
Concen: 51.328 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27

Tgt Ion: 95 Resp: 146744
Ion Ratio Lower Upper
95 100
174 73.9 0.0 141.8
176 70.2 0.0 138.2


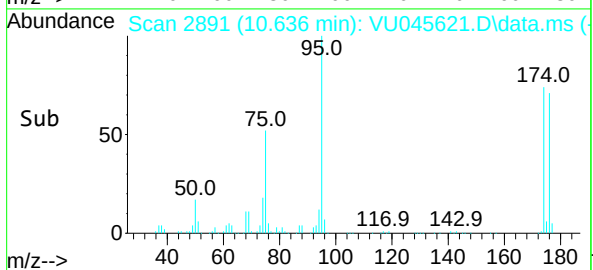
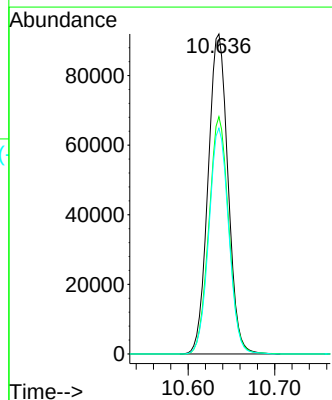
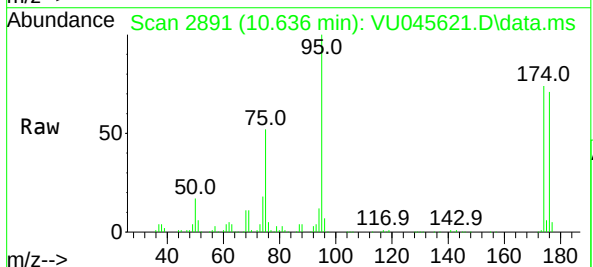


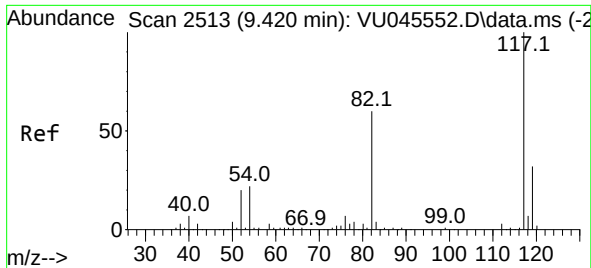

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27

Instrument :
MSVOA_U
ClientSampleId :
TRIP-BLANK

Tgt Ion:117 Resp: 289414
Ion Ratio Lower Upper
117 100
82 58.5 47.8 71.8
119 32.4 25.8 38.8

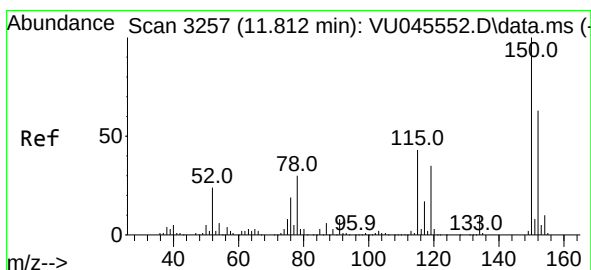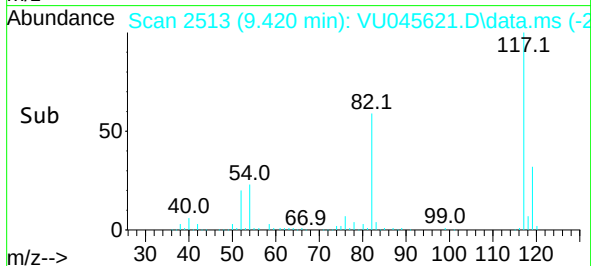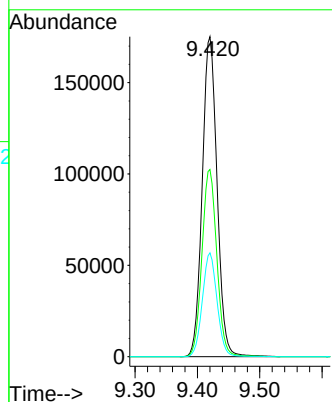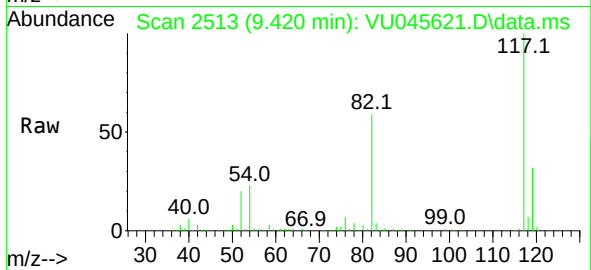

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU045621.D
Acq: 08 Nov 2021 17:27

Tgt Ion:152 Resp: 147893
Ion Ratio Lower Upper
152 100
115 61.4 42.7 128.1
150 157.9 0.0 346.8

