

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
 Data File : VU045632.D
 Acq On : 08 Nov 2021 22:27
 Operator : SY/MD
 Sample : VU1108WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1108WBL02

Quant Time: Nov 09 10:06:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.376	168	153460	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	283233	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	287092	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.813	152	145493	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.707	65	120864	52.590	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	105.180%
35) Dibromofluoromethane	5.292	113	94867	50.168	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.340%
50) Toluene-d8	7.900	98	371539	52.838	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	105.680%
62) 4-Bromofluorobenzene	10.636	95	143056	50.735	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045632.D
Acq On : 08 Nov 2021 22:27
Operator : SY/MD
Sample : VU1108WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1108WBL02

Quant Time: Nov 09 10:06:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 05 13:35:16 2021
Response via : Initial Calibration




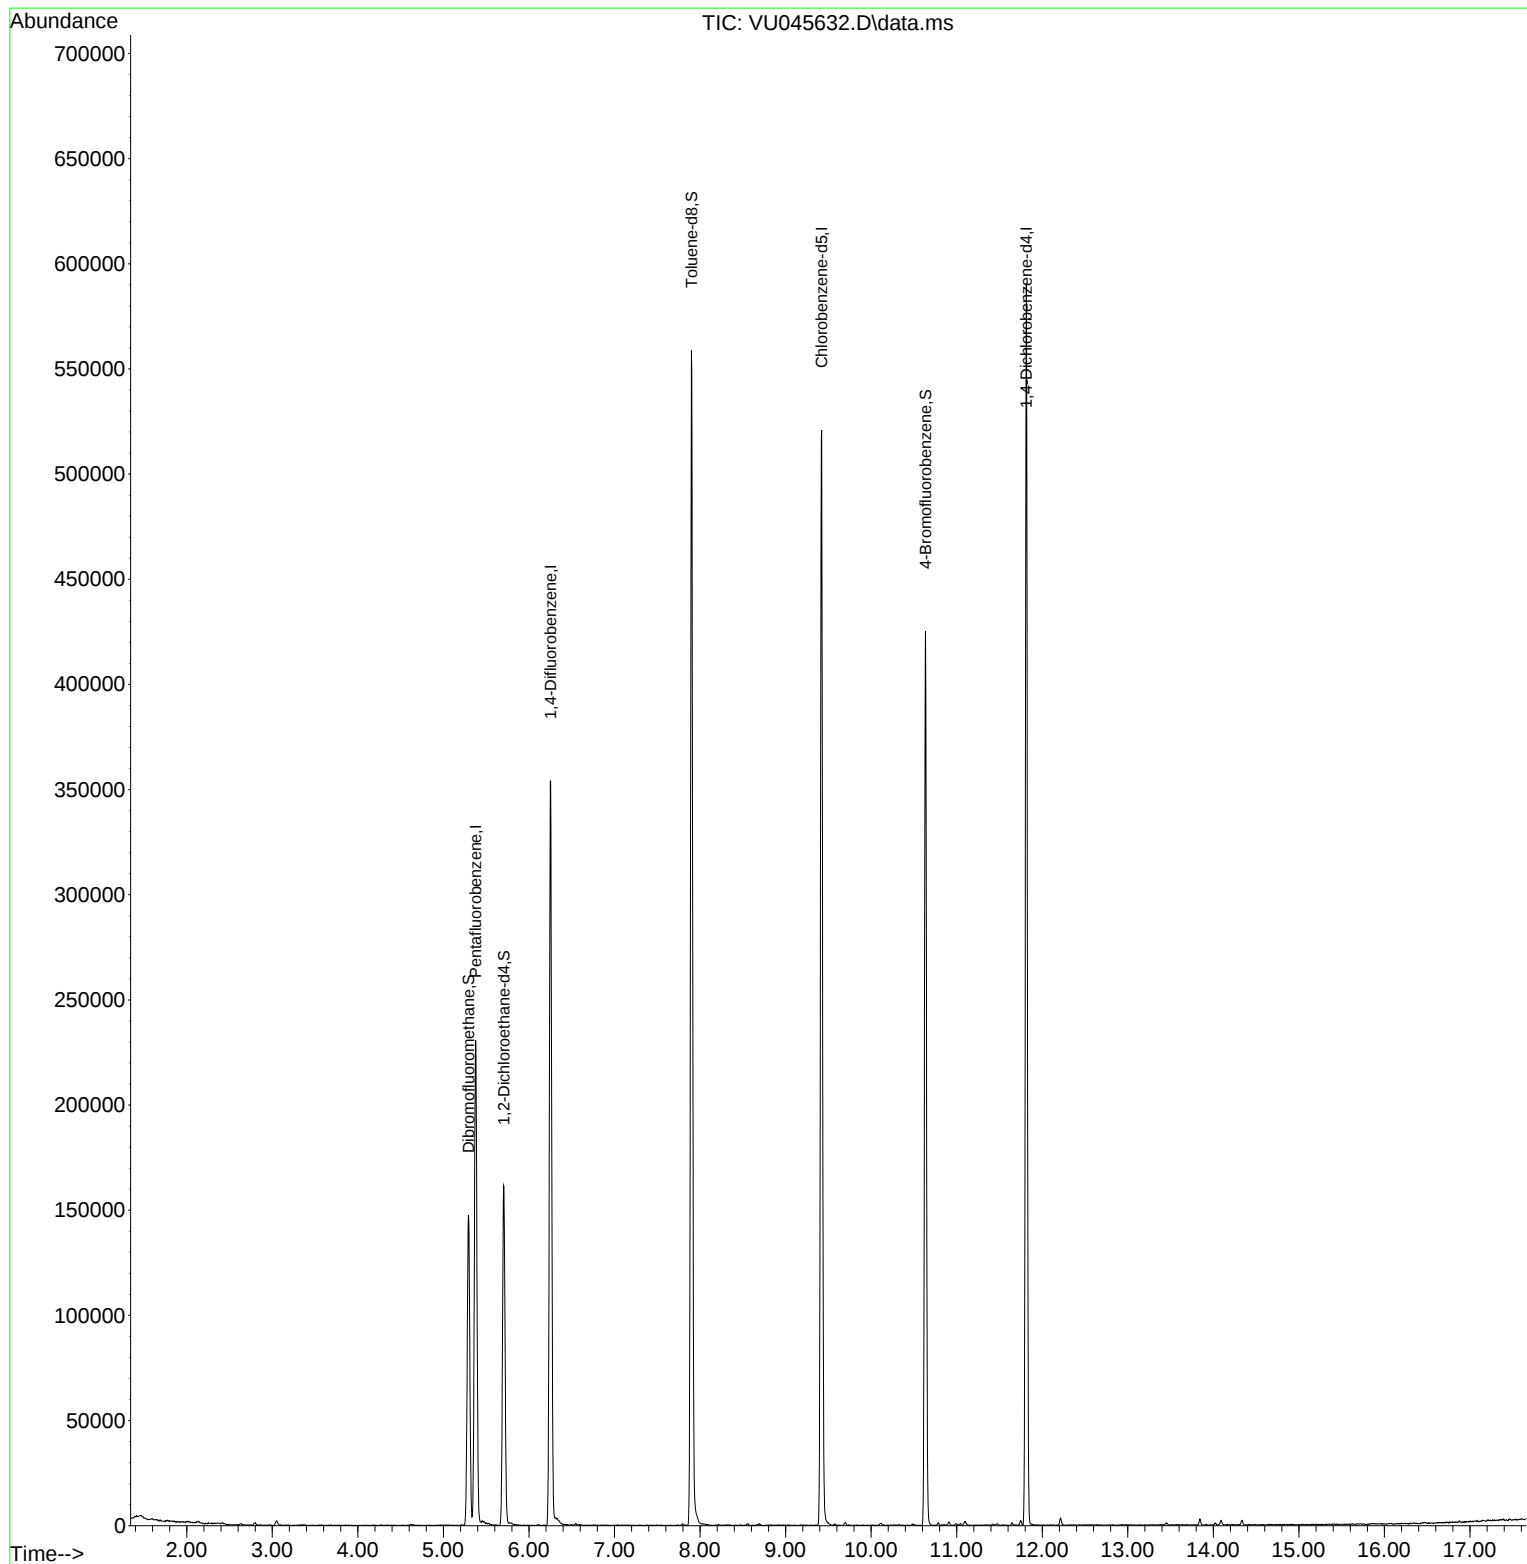


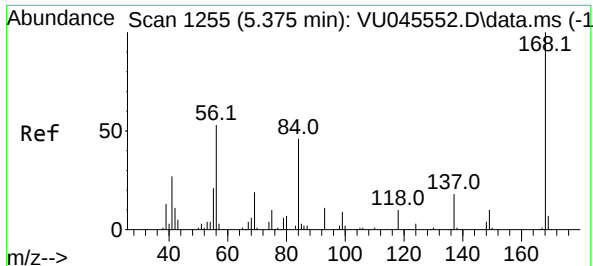

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.376 min Scan# 11
Delta R.T. 0.001 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27




Instrument :
MSVOA_U
ClientSampleId :
VU1108WBL02


Tgt Ion:168 Resp: 153460
Ion Ratio Lower Upper
168 100
99 62.8 51.0 76.6

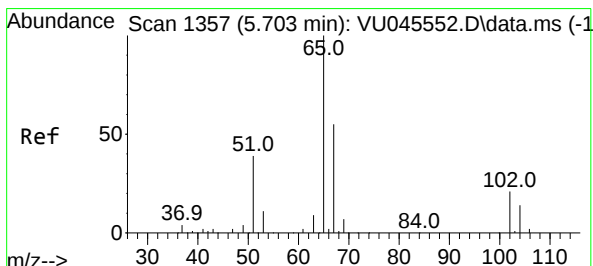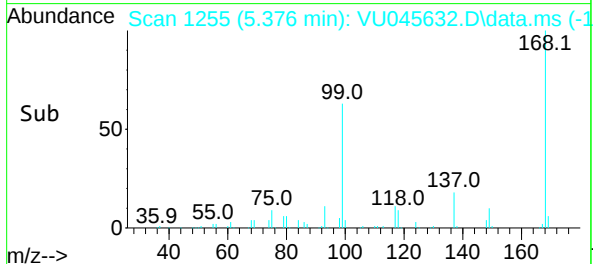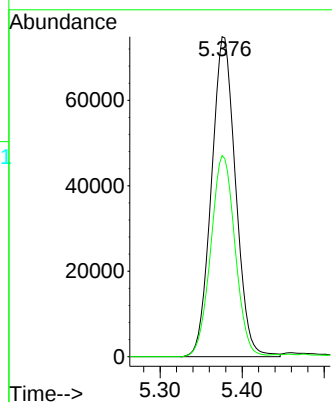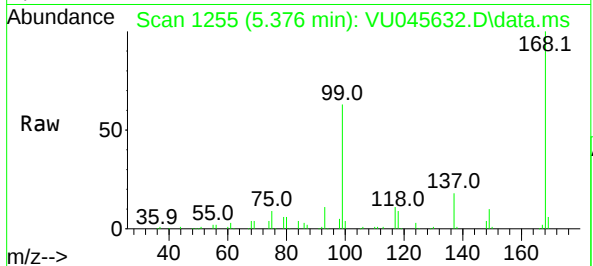

#33
1,2-Dichloroethane-d4
Concen: 52.590 ug/l
RT: 5.707 min Scan# 1358
Delta R.T. 0.003 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27

Tgt Ion: 65 Resp: 120864
Ion Ratio Lower Upper
65 100
67 53.1 0.0 105.8

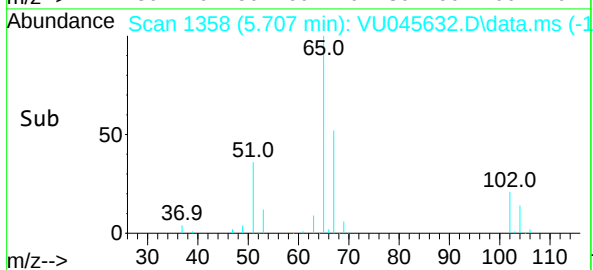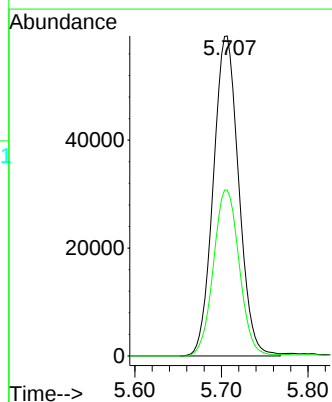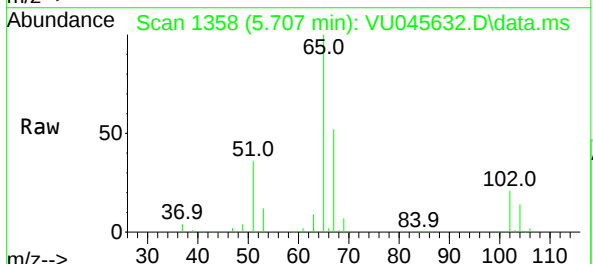

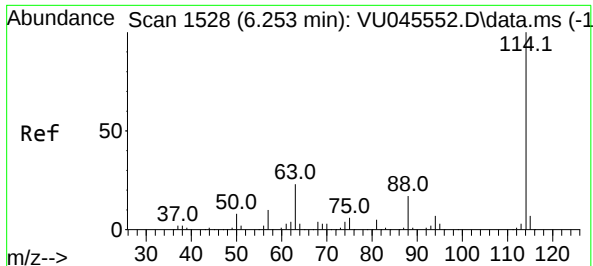

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU045632.D

Acq: 08 Nov 2021 22:27

Instrument :

MSVOA_U

ClientSampleId :

VU1108WBL02





Tgt Ion:114 Resp: 283233

Ion Ratio Lower Upper

114 100

63 21.2 0.0 45.6

88 16.7 0.0 33.8

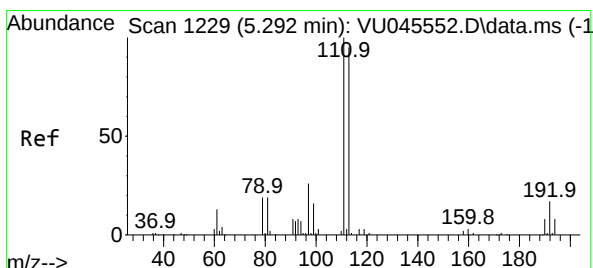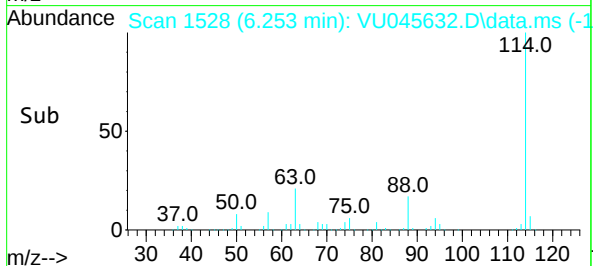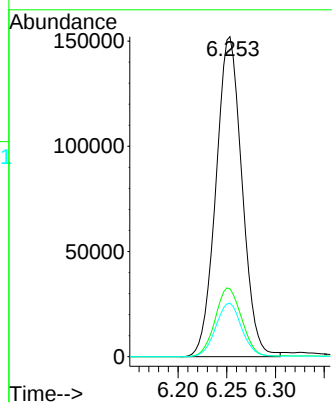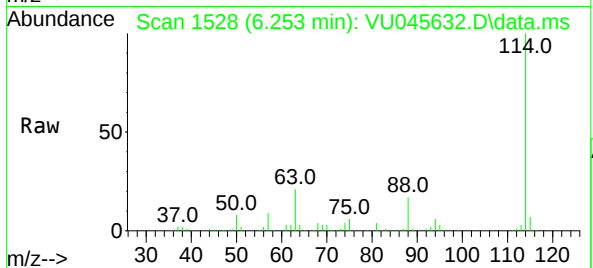

#35

Dibromofluoromethane

Concen: 50.168 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. 0.000 min

Lab File: VU045632.D

Acq: 08 Nov 2021 22:27




Tgt Ion:113 Resp: 94867


Ion Ratio Lower Upper

113 100

111 103.0 82.8 124.2

192 18.8 14.8 22.2


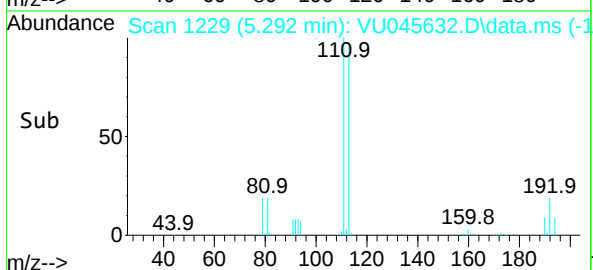
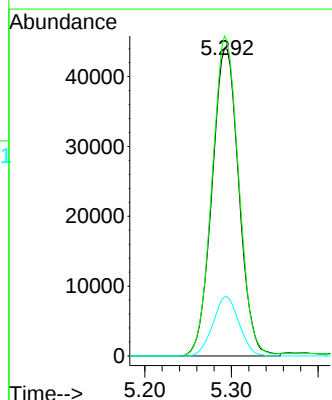
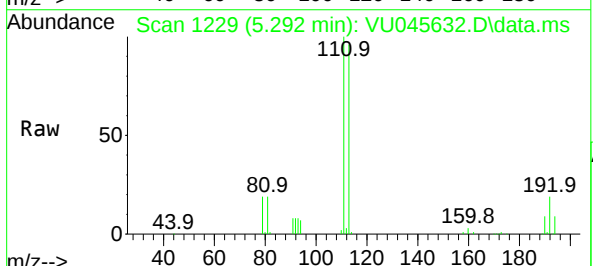


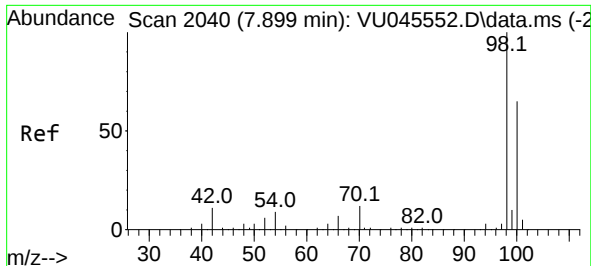

#50
Toluene-d8
Concen: 52.838 ug/l
RT: 7.900 min Scan# 2040
Delta R.T. 0.000 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27




Instrument :
MSVOA_U
ClientSampleId :
VU1108WBL02


Tgt Ion: 98 Resp: 371539
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

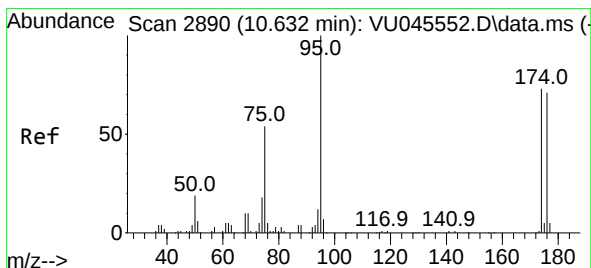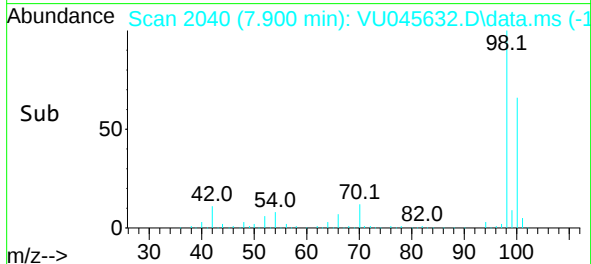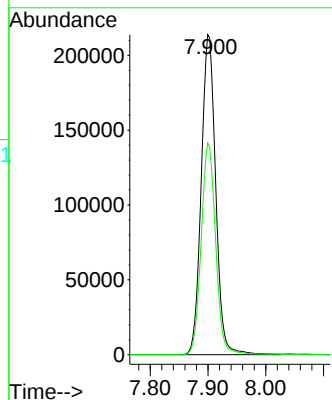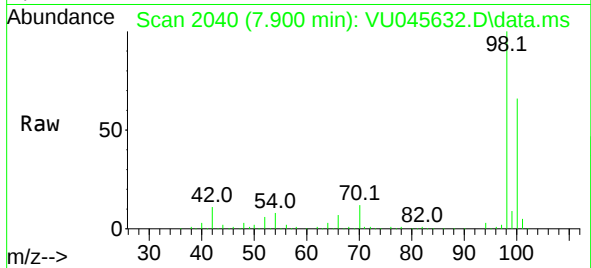

#62
4-Bromofluorobenzene
Concen: 50.735 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27

Tgt Ion: 95 Resp: 143056
Ion Ratio Lower Upper
95 100
174 75.8 0.0 141.8
176 72.0 0.0 138.2


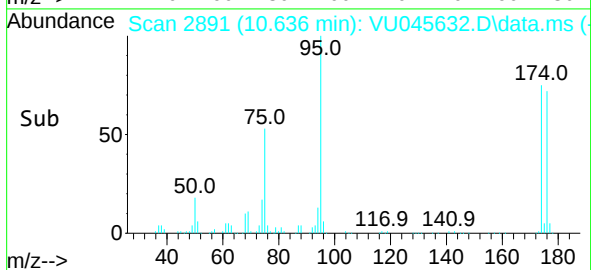
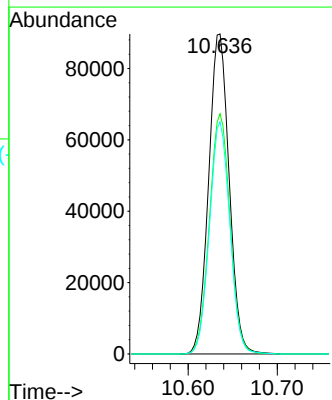
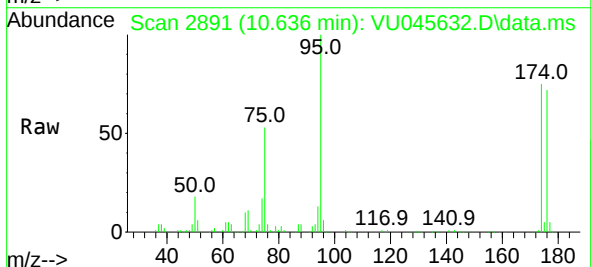


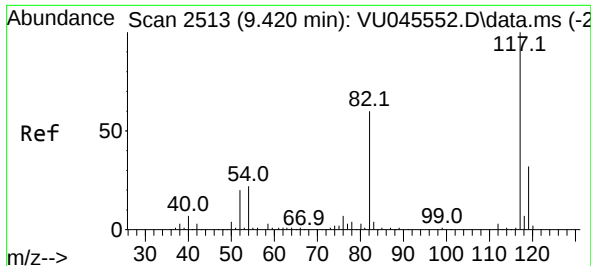

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27

Instrument :
MSVOA_U
ClientSampleId :
VU1108WBL02

Tgt Ion:117 Resp: 287092
Ion Ratio Lower Upper
117 100
82 59.2 47.8 71.8
119 31.6 25.8 38.8

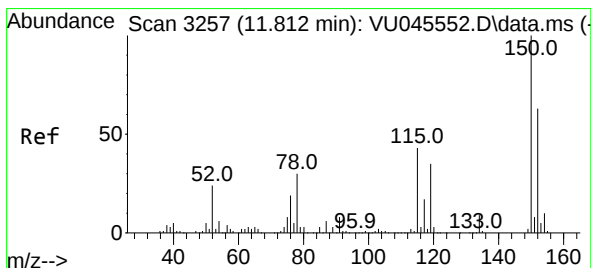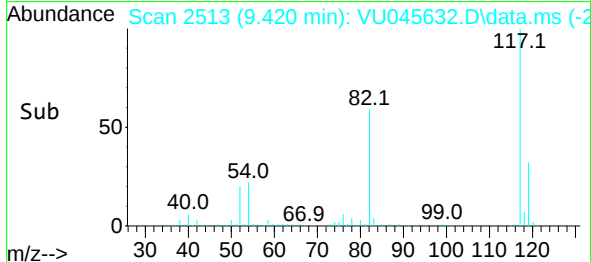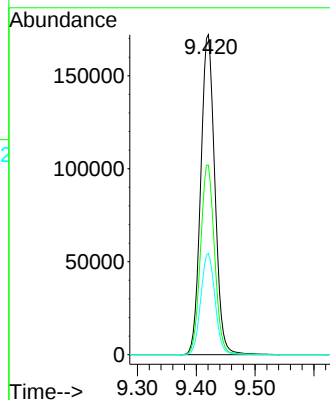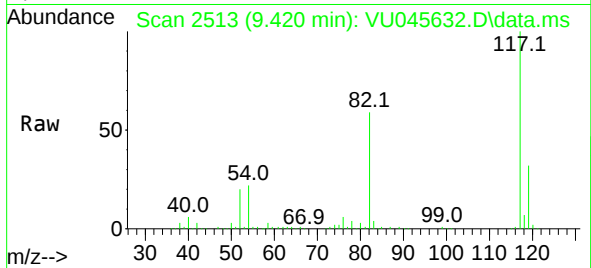

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.813 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU045632.D
Acq: 08 Nov 2021 22:27

Tgt Ion:152 Resp: 145493
Ion Ratio Lower Upper
152 100
115 62.0 42.7 128.1
150 157.3 0.0 346.8

