

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
 Data File : VU045638.D
 Acq On : 09 Nov 2021 00:45
 Operator : SY/MD
 Sample : M4495-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DRW-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260

Signal : TIC: VU045638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.292	1214	1229	1243	rBV	146967	313306	32.19%	5.749%
2	5.375	1243	1255	1278	rVB	226645	463454	47.61%	8.504%
3	5.703	1341	1357	1374	rBV	164703	332610	34.17%	6.103%
4	6.253	1513	1528	1546	rBV	356954	673822	69.22%	12.364%
5	7.899	2026	2040	2064	rBV	561869	973422	100.00%	17.861%
6	9.420	2499	2513	2548	rVB	538355	886079	91.03%	16.259%
7	10.636	2877	2891	2915	rBV	441482	691281	71.02%	12.684%
8	11.812	3243	3257	3277	rBV	610879	949603	97.55%	17.424%
9	13.459	3759	3769	3778	rVB4	10821	16557	1.70%	0.304%
10	13.841	3877	3888	3896	rBV4	7737	11380	1.17%	0.209%
11	13.941	3914	3919	3930	rVB2	9280	13822	1.42%	0.254%
12	14.192	3989	3997	4008	rVB2	10749	15705	1.61%	0.288%
13	14.288	4018	4027	4036	rVB3	10220	14540	1.49%	0.267%
14	14.668	4132	4145	4160	rBV4	6697	12093	1.24%	0.222%
15	14.880	4201	4211	4220	rVV4	7199	11165	1.15%	0.205%
16	15.021	4246	4255	4267	rBV4	12493	22401	2.30%	0.411%
17	15.201	4301	4311	4320	rBV4	8590	14081	1.45%	0.258%
18	15.275	4326	4334	4344	rVB4	6299	10148	1.04%	0.186%
19	15.597	4418	4434	4443	rVB4	3925	9900	1.02%	0.182%
20	15.928	4529	4537	4552	rVB5	7643	14521	1.49%	0.266%




Sum of corrected areas: 5449890

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045638.D
Acq On : 09 Nov 2021 00:45
Operator : SY/MD
Sample : M4495-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DRW-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

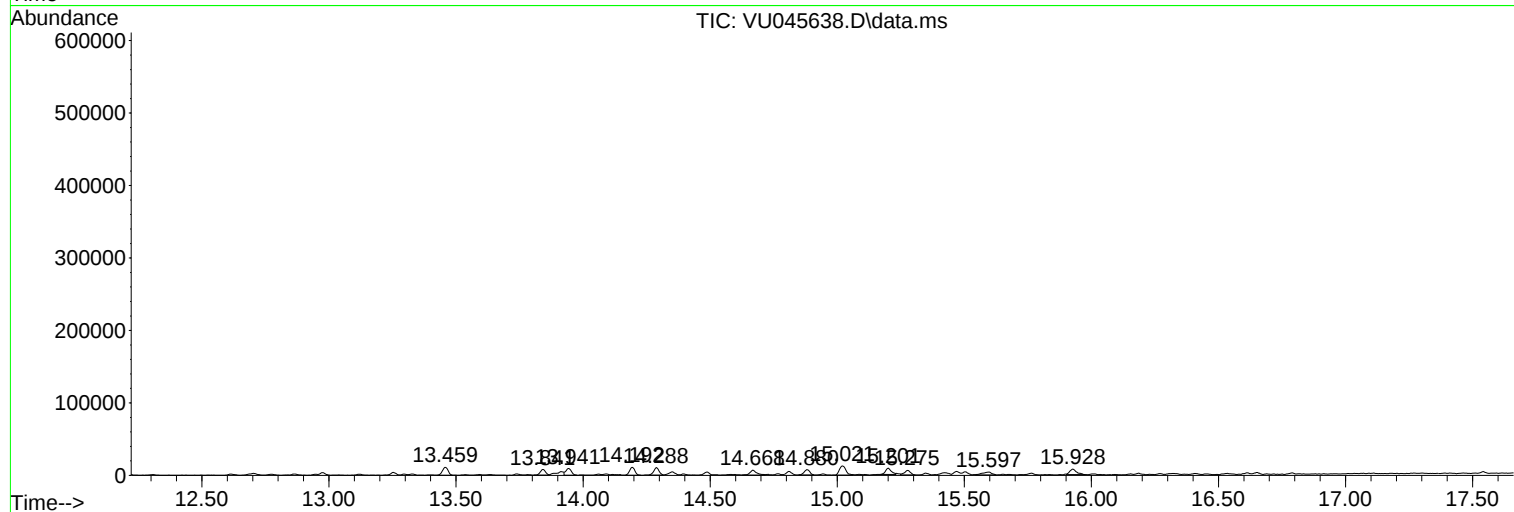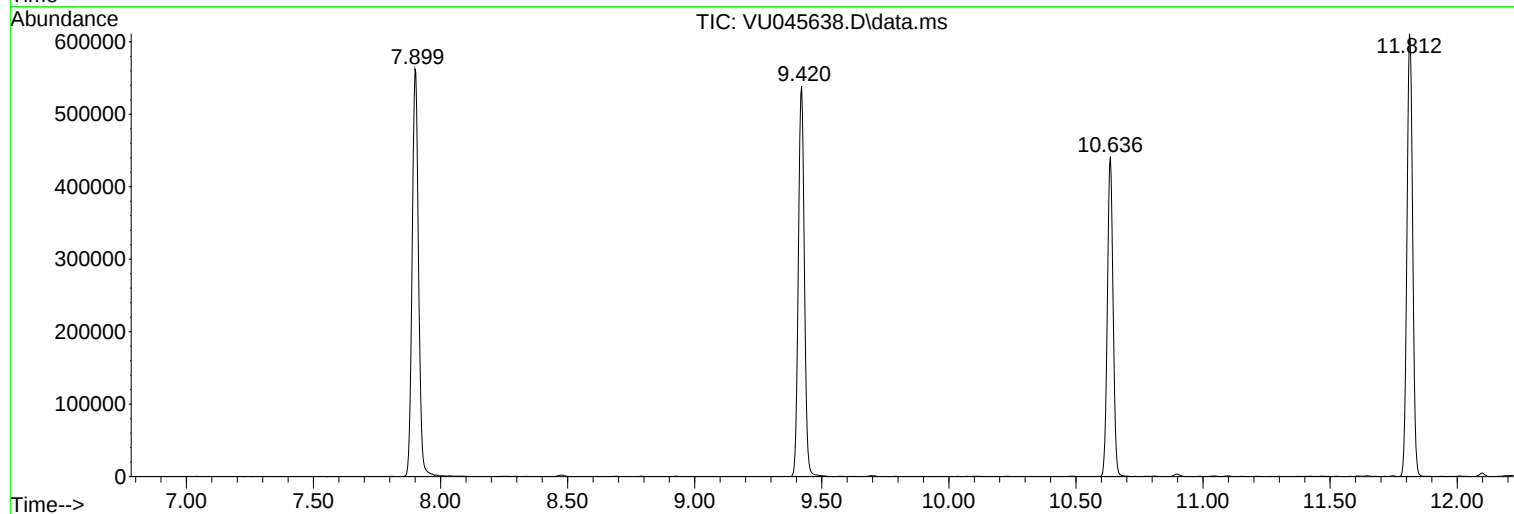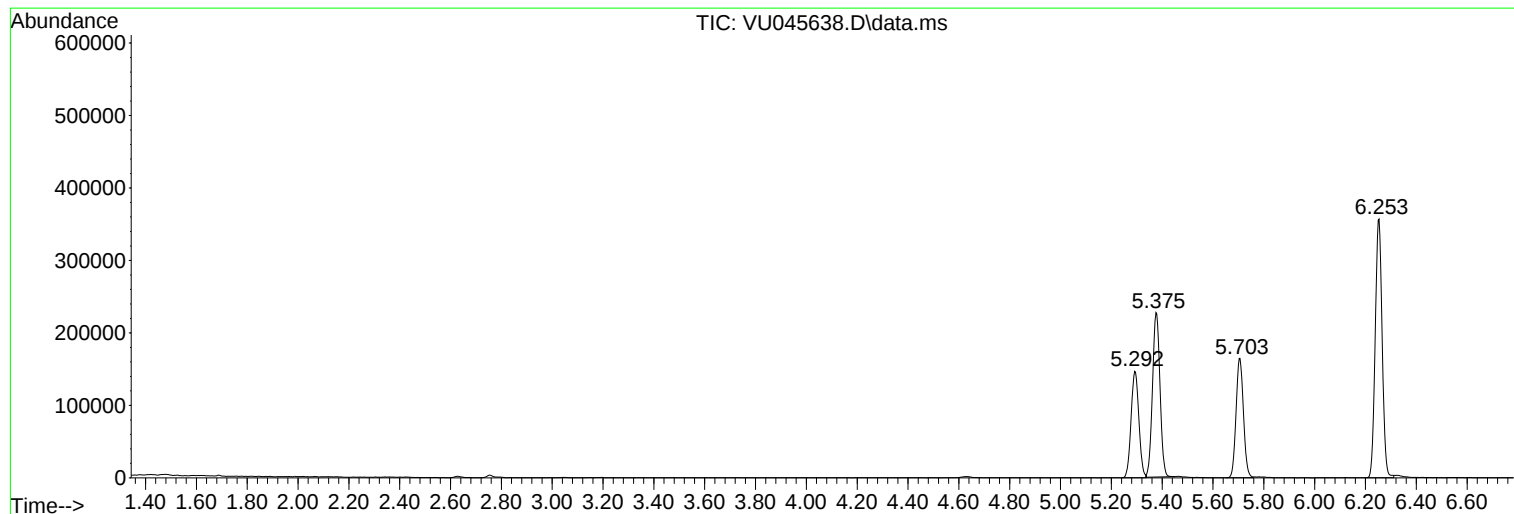

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045638.D
Acq On : 09 Nov 2021 00:45
Operator : SY/MD
Sample : M4495-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DRW-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045638.D
Acq On : 09 Nov 2021 00:45
Operator : SY/MD
Sample : M4495-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DRW-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------