


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045600.D
Acq On : 08 Nov 2021 08:55
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Title : SW846 8260
Last Update : Fri Nov 05 13:35:16 2021

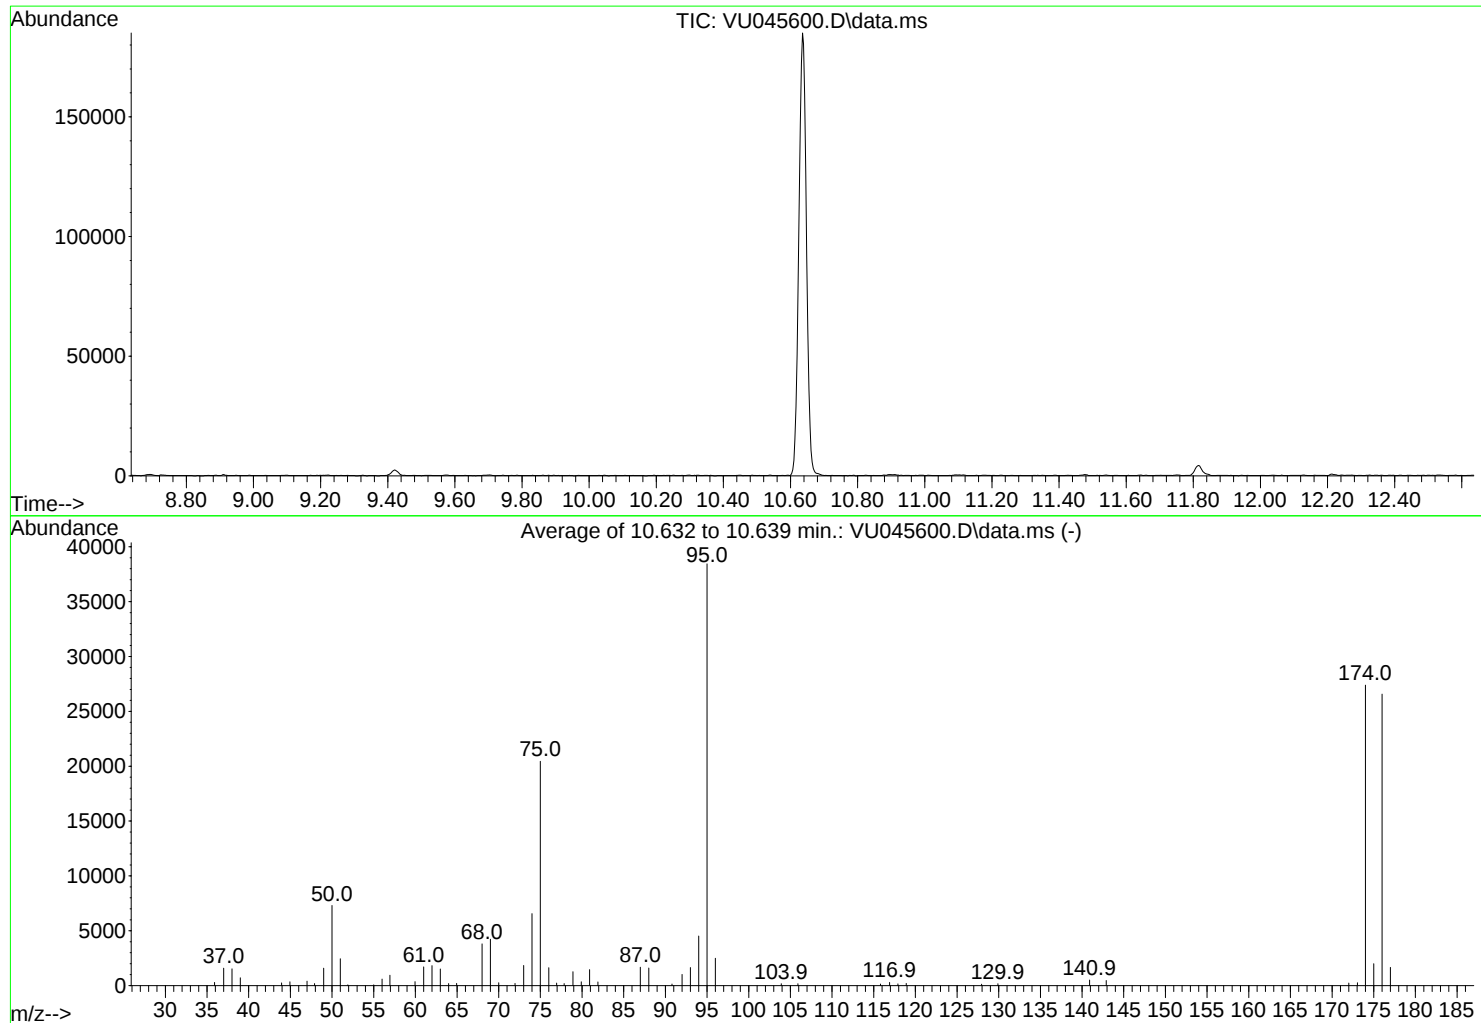

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	7313	PASS
75	95	30	60	53.2	20451	PASS
95	95	100	100	100.0	38445	PASS
96	95	5	9	6.5	2499	PASS
173	174	0.00	2	1.0	268	PASS
174	95	50	100	71.2	27392	PASS
175	174	5	9	7.3	1992	PASS
176	174	95	101	97.0	26576	PASS
177	176	5	9	6.3	1665	PASS