
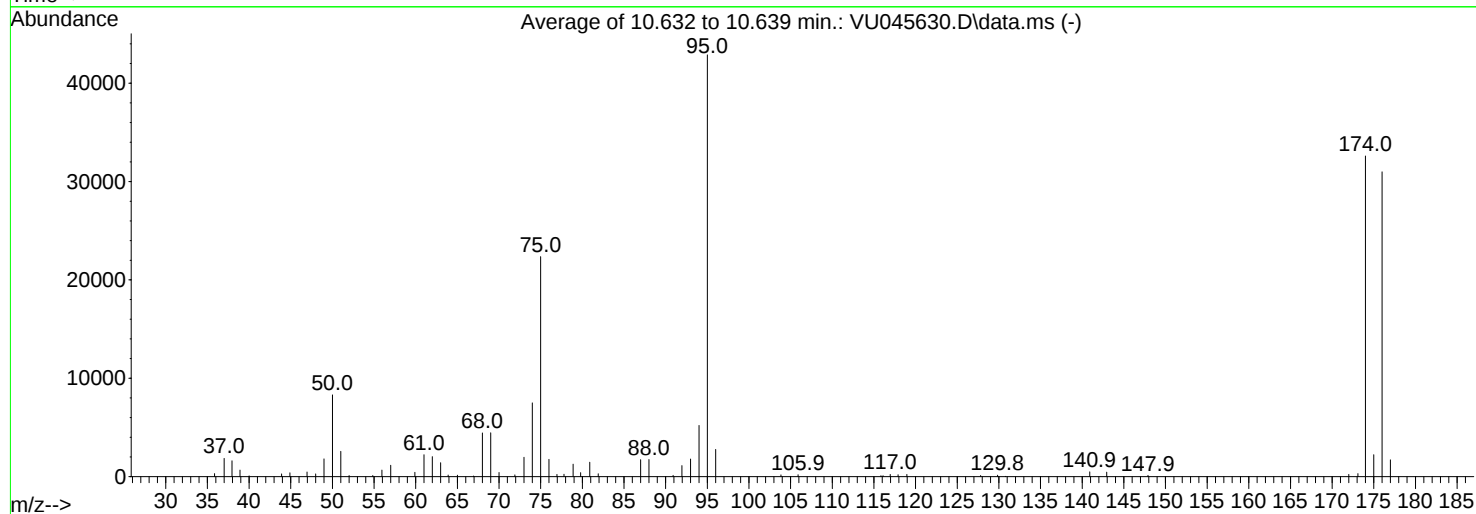


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110821\
Data File : VU045630.D
Acq On : 08 Nov 2021 20:55
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Title : SW846 8260
Last Update : Fri Nov 05 13:35:16 2021

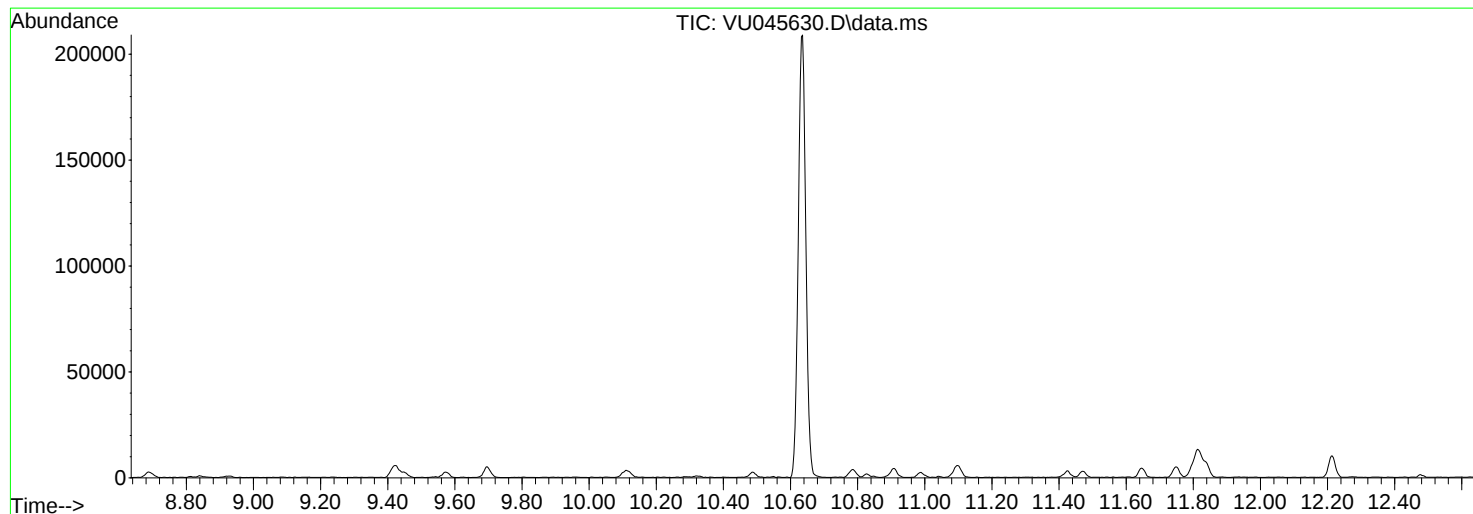

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	8307	PASS
75	95	30	60	52.2	22373	PASS
95	95	100	100	100.0	42880	PASS
96	95	5	9	6.5	2767	PASS
173	174	0.00	2	1.0	311	PASS
174	95	50	100	76.0	32600	PASS
175	174	5	9	6.8	2228	PASS
176	174	95	101	95.0	30984	PASS
177	176	5	9	5.5	1711	PASS