

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
 Data File : VU061557.D
 Acq On : 08 Nov 2024 19:02
 Operator : MD/SY
 Sample : P4748-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP58

Quant Time: Nov 09 00:22:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 09 00:17:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	159649	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	152454	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	64019	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	40063	3.694	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.800%
7) Chloroethane-d5	1.911	69	42391	4.264	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.200%
11) 1,1-Dichloroethene-d2	2.560	65	19614	4.227	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	4.624	46	110299	50.094	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.180%
24) Chloroform-d	5.052	84	94225	4.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.692	65	49211	4.796	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	5.717	84	192388	4.479	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	6.682	67	59513	4.608	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%
41) Toluene-d8	7.891	98	169107	4.210	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	8.174	79	17426	3.305	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.200%
46) 2-Hexanone-d5	8.627	63	96704	44.787	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.580%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	46409	4.752	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	56152	4.953	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds					Qvalue	
13) Acetone	2.644	43	13005	9.325	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061557.D
Acq On : 08 Nov 2024 19:02
Operator : MD/SY
Sample : P4748-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP58


Quant Time: Nov 09 00:22:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 09 00:17:10 2024
Response via : Initial Calibration

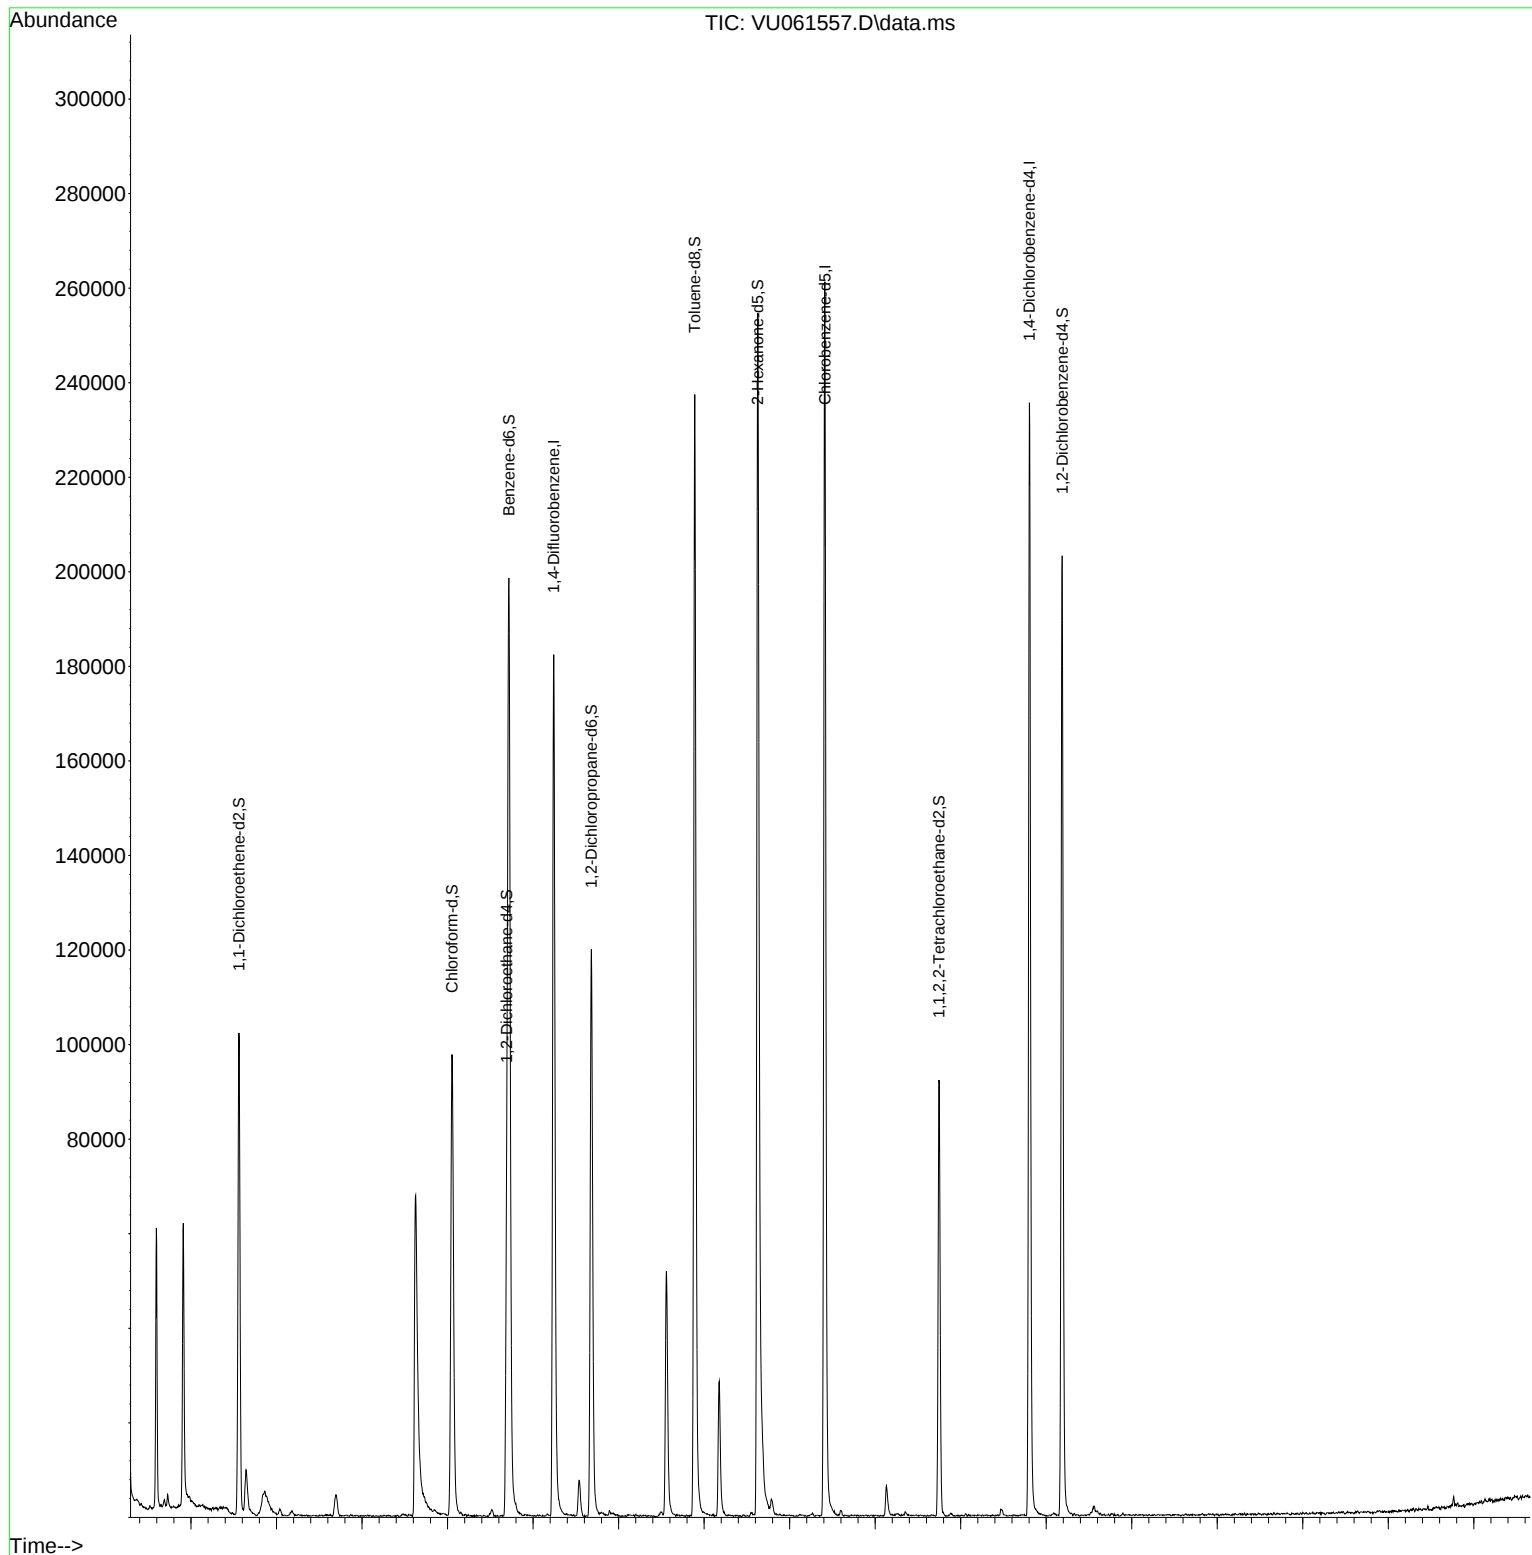

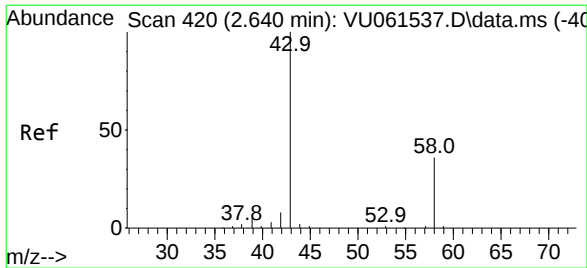

#13
 Acetone
 Concen: 9.325 ug/L
 RT: 2.644 min Scan# 42
 Delta R.T. 0.003 min
 Lab File: VU061557.D
 Acq: 08 Nov 2024 19:02

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP58

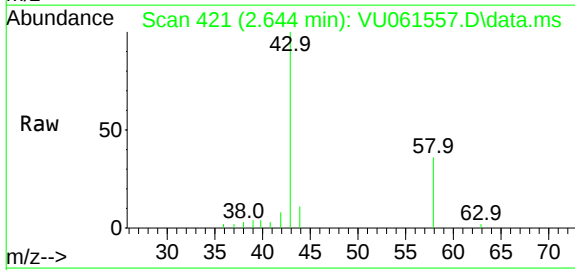

Tgt Ion: 43 Resp: 13005
 Ion Ratio Lower Upper
 43 100
 58 36.9 0.0 73.2

