

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
 Data File : VU061544.D
 Acq On : 08 Nov 2024 13:13
 Operator : MD/SY
 Sample : P4743-06DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H46R5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	15	21	36	rVB4	7553	10225	1.82%	0.200%
2	1.596	69	95	110	rBV2	98038	190741	33.89%	3.728%
3	1.908	185	192	208	rVB	64643	86789	15.42%	1.696%
4	2.560	382	395	413	rBV	107605	178956	31.79%	3.498%
5	3.174	573	586	600	rBV2	4577	10306	1.83%	0.201%
6	3.348	630	640	657	rBV2	12194	25123	4.46%	0.491%
7	3.695	736	748	762	rVB3	5441	12451	2.21%	0.243%
8	4.653	1024	1046	1101	rBV2	171283	562849	100.00%	11.002%
9	5.052	1155	1170	1190	rBV	102226	229365	40.75%	4.483%
10	5.714	1358	1376	1405	rBV2	204054	540005	95.94%	10.555%
11	6.242	1528	1540	1568	rBV	206275	402709	71.55%	7.872%
12	6.538	1623	1632	1645	rBV4	7781	16064	2.85%	0.314%
13	6.682	1664	1677	1703	rBV	124547	248531	44.16%	4.858%
14	7.560	1937	1950	1971	rBV	55956	102819	18.27%	2.010%
15	7.891	2041	2053	2072	rBV	248737	441713	78.48%	8.634%
16	8.174	2131	2141	2162	rBV2	31148	56287	10.00%	1.100%
17	8.628	2271	2282	2327	rBV	265967	536197	95.26%	10.481%
18	9.409	2513	2525	2557	rBV	289708	508222	90.29%	9.934%
19	10.746	2931	2941	2960	rBV	95221	155081	27.55%	3.031%
20	11.804	3259	3270	3294	rBV	260744	440212	78.21%	8.605%
21	12.187	3375	3389	3413	rBV	211513	361229	64.18%	7.061%




Sum of corrected areas: 5115874

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061544.D
Acq On : 08 Nov 2024 13:13
Operator : MD/SY
Sample : P4743-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46R5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

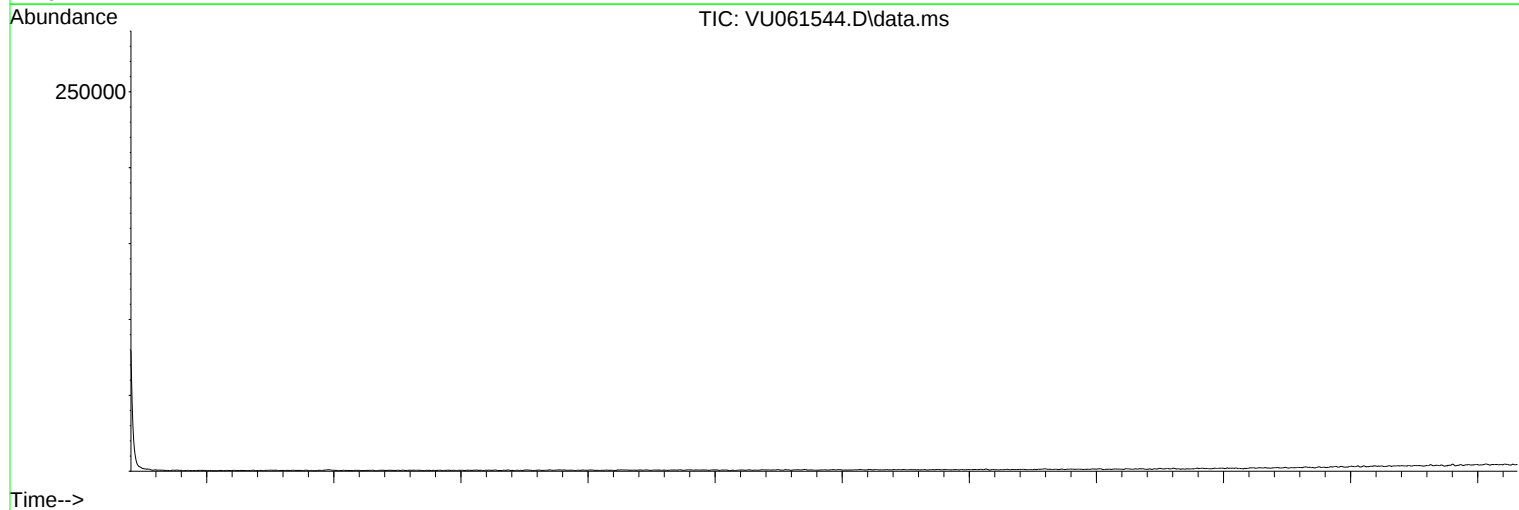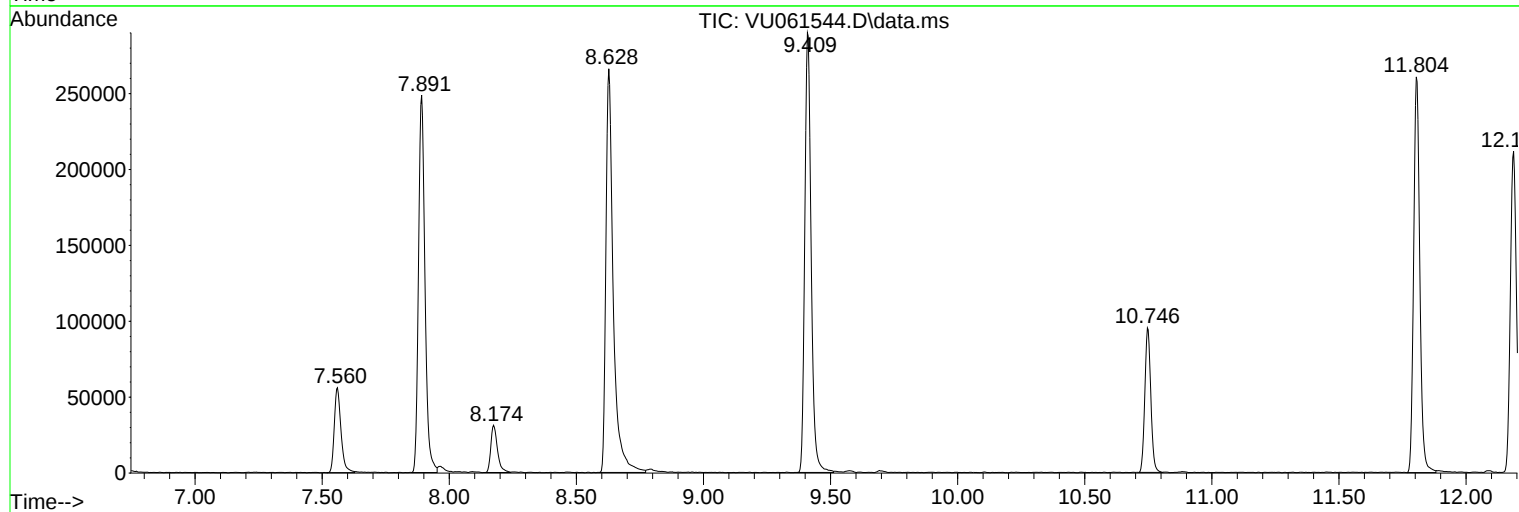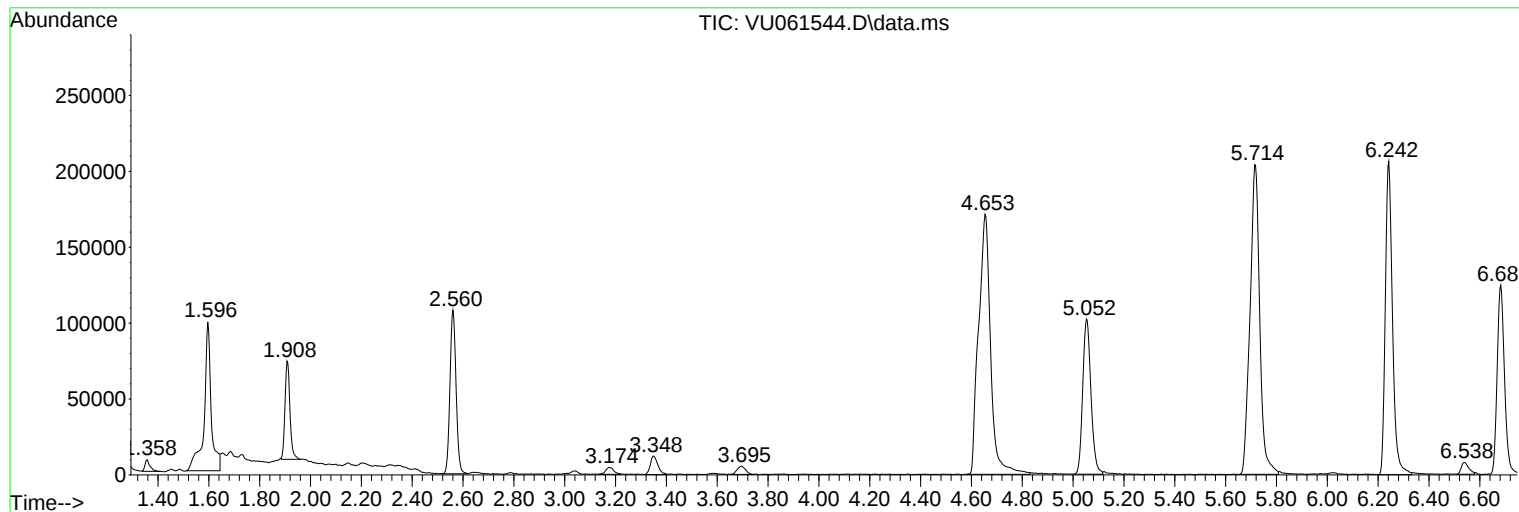

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061544.D
Acq On : 08 Nov 2024 13:13
Operator : MD/SY
Sample : P4743-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46R5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061544.D
Acq On : 08 Nov 2024 13:13
Operator : MD/SY
Sample : P4743-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46R5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------