

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
 Data File : VU061550.D
 Acq On : 08 Nov 2024 15:40
 Operator : MD/SY
 Sample : P4743-13DL 10X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H46S7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	85	96	111	rBV2	117987	160522	26.33%	2.870%
2	1.907	183	192	207	rBV	65876	119890	19.66%	2.144%
3	2.550	380	392	413	rVB	118626	196784	32.27%	3.519%
4	3.036	533	543	552	rBV3	4025	6898	1.13%	0.123%
5	3.177	574	587	608	rVB	13647	34258	5.62%	0.613%
6	3.351	629	641	660	rBV5	10951	26648	4.37%	0.476%
7	3.682	730	744	767	rBV2	39672	90464	14.84%	1.618%
8	4.653	1026	1046	1094	rBV2	148011	471476	77.33%	8.430%
9	5.052	1152	1170	1198	rBV	109413	250668	41.11%	4.482%
10	5.714	1356	1376	1408	rBV2	232918	603470	98.98%	10.790%
11	6.238	1527	1539	1573	rBV	229163	450570	73.90%	8.056%
12	6.682	1663	1677	1700	rBV	137800	273750	44.90%	4.895%
13	7.560	1939	1950	1979	rBV	58158	109040	17.88%	1.950%
14	7.891	2041	2053	2077	rBV	279487	496630	81.45%	8.880%
15	8.177	2131	2142	2162	rBV2	32948	61159	10.03%	1.094%
16	8.640	2274	2286	2325	rBV	263328	609716	100.00%	10.902%
17	9.412	2514	2526	2554	rBV	318502	560168	91.87%	10.016%
18	10.753	2930	2943	2962	rBV	104166	173742	28.50%	3.107%
19	11.807	3259	3271	3291	rBV	301234	492187	80.72%	8.801%
20	12.187	3375	3389	3412	rBV	240277	404622	66.36%	7.235%

Sum of corrected areas: 5592662




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061550.D
Acq On : 08 Nov 2024 15:40
Operator : MD/SY
Sample : P4743-13DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46S7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

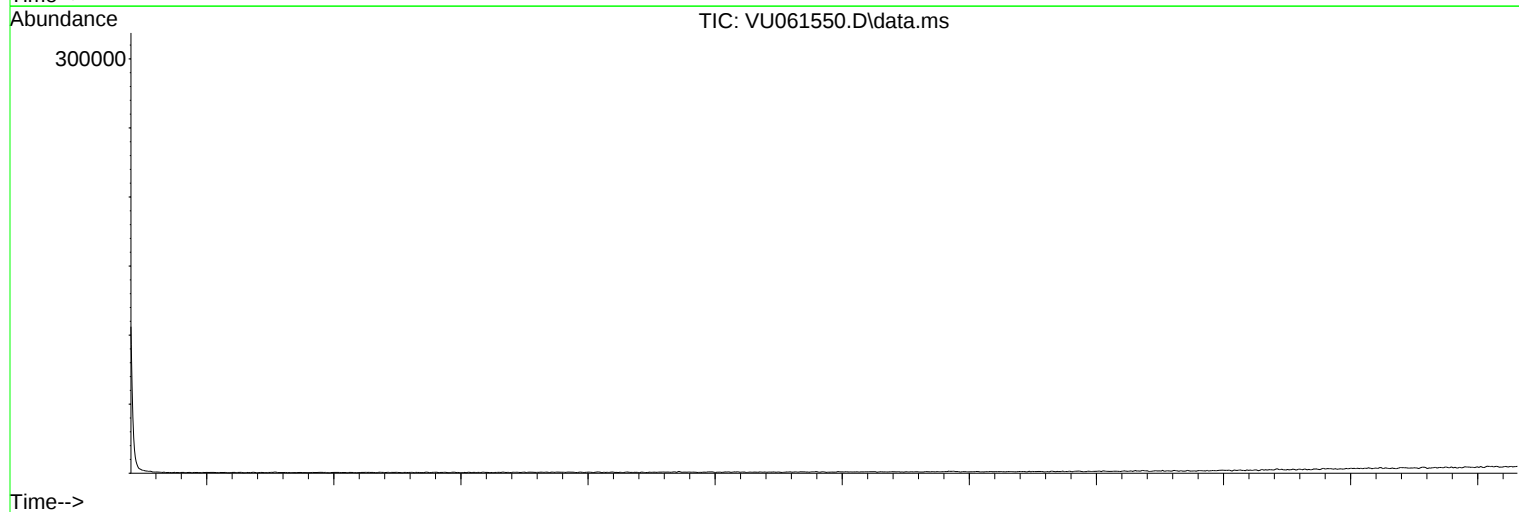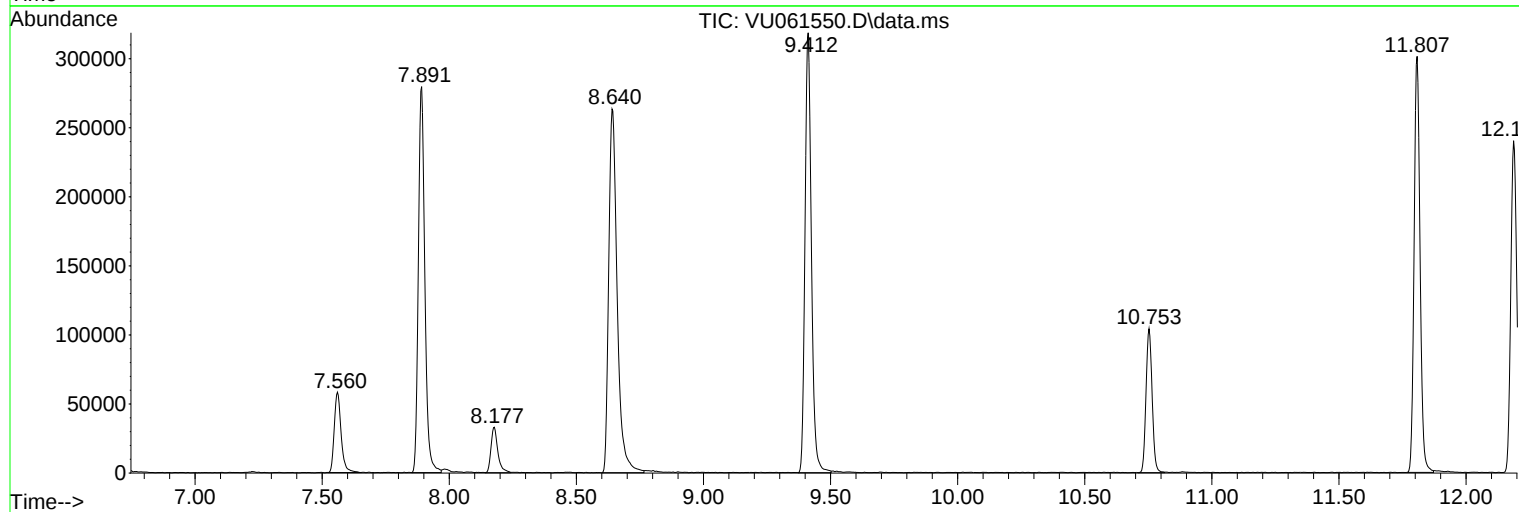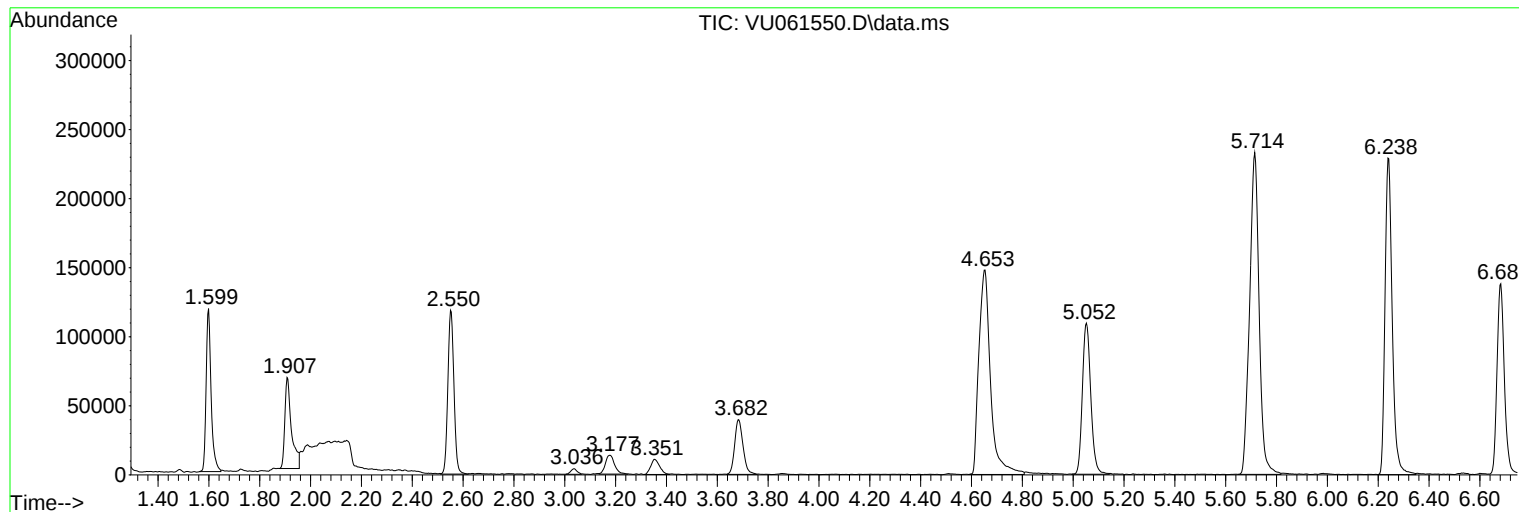

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061550.D
Acq On : 08 Nov 2024 15:40
Operator : MD/SY
Sample : P4743-13DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46S7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Ethyl-oxetane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.682	1.00 ug/L	90464	1,4-Difluorobenzene	6.242

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Ethyl-oxetane	86	C5H10O	1010386-40-2	91
2	n-Hexane	86	C6H14	000110-54-3	90
3	n-Hexane	86	C6H14	000110-54-3	72
4	n-Hexane	86	C6H14	000110-54-3	72
5	n-Hexane	86	C6H14	000110-54-3	72

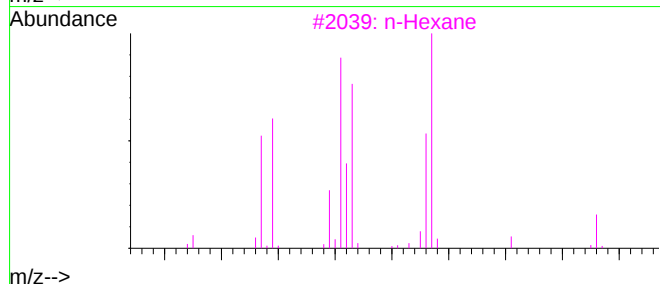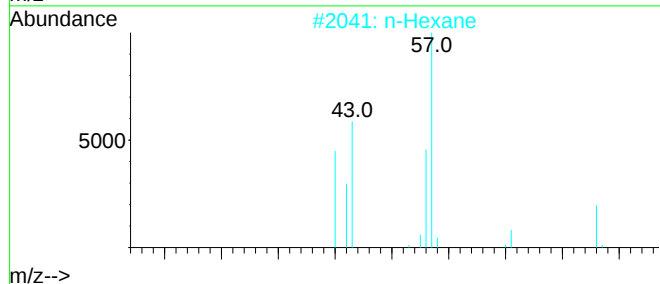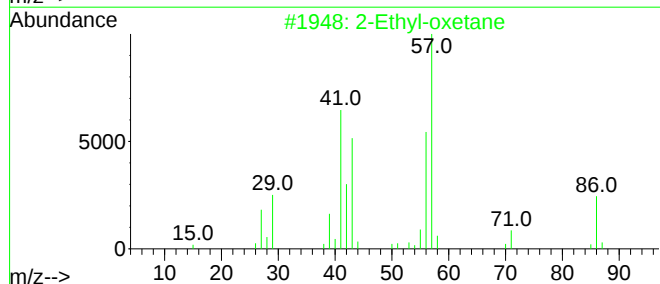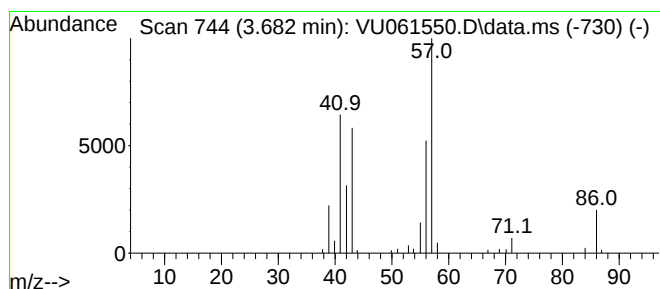

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110824\
Data File : VU061550.D
Acq On : 08 Nov 2024 15:40
Operator : MD/SY
Sample : P4743-13DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46S7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Ethyl-oxetane	3.682	1.0	ug/L	90464	1	6.242	450570	5.0