

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111123\  
 Data File : VU056212.D  
 Acq On : 11 Nov 2023 13:13  
 Operator : MD/SY  
 Sample : 05340-06  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCDL1

Quant Time: Nov 11 20:21:15 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR110723WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Nov 11 20:19:10 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	372522	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	372238	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	172436	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	93129	4.028	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	80.600%	
7) Chloroethane-d5	1.911	69	78525	5.004	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	100.000%	
11) 1,1-Dichloroethene-d2	2.563	65	43823	4.302	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	86.000%	
20) 2-Butanone-d5	4.621	46	270877	71.408	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	142.820%#	
24) Chloroform-d	5.058	84	224717	5.105	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
26) 1,2-Dichloroethane-d4	5.695	65	108764	5.612	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	112.200%	
32) Benzene-d6	5.724	84	442200	4.946	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6	6.685	67	142461	5.413	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.200%	
41) Toluene-d8	7.894	98	365154	4.457	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.200%	
43) trans-1,3-Dichloroprop...	8.177	79	48717	4.843	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.800%	
46) 2-Hexanone-d5	8.631	63	232531	70.525	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	141.060%#	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	111356	5.928	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	118.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152	146931	5.525	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
-----						
Target Compounds						Qvalue
13) Acetone	2.631	43	27058	9.672	ug/L	98
-----						


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111123\  
 Data File : VU056212.D  
 Acq On : 11 Nov 2023 13:13  
 Operator : MD/SY  
 Sample : 05340-06  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCGL1

Quant Time: Nov 11 20:21:15 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR110723WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Nov 11 20:19:10 2023  
 Response via : Initial Calibration

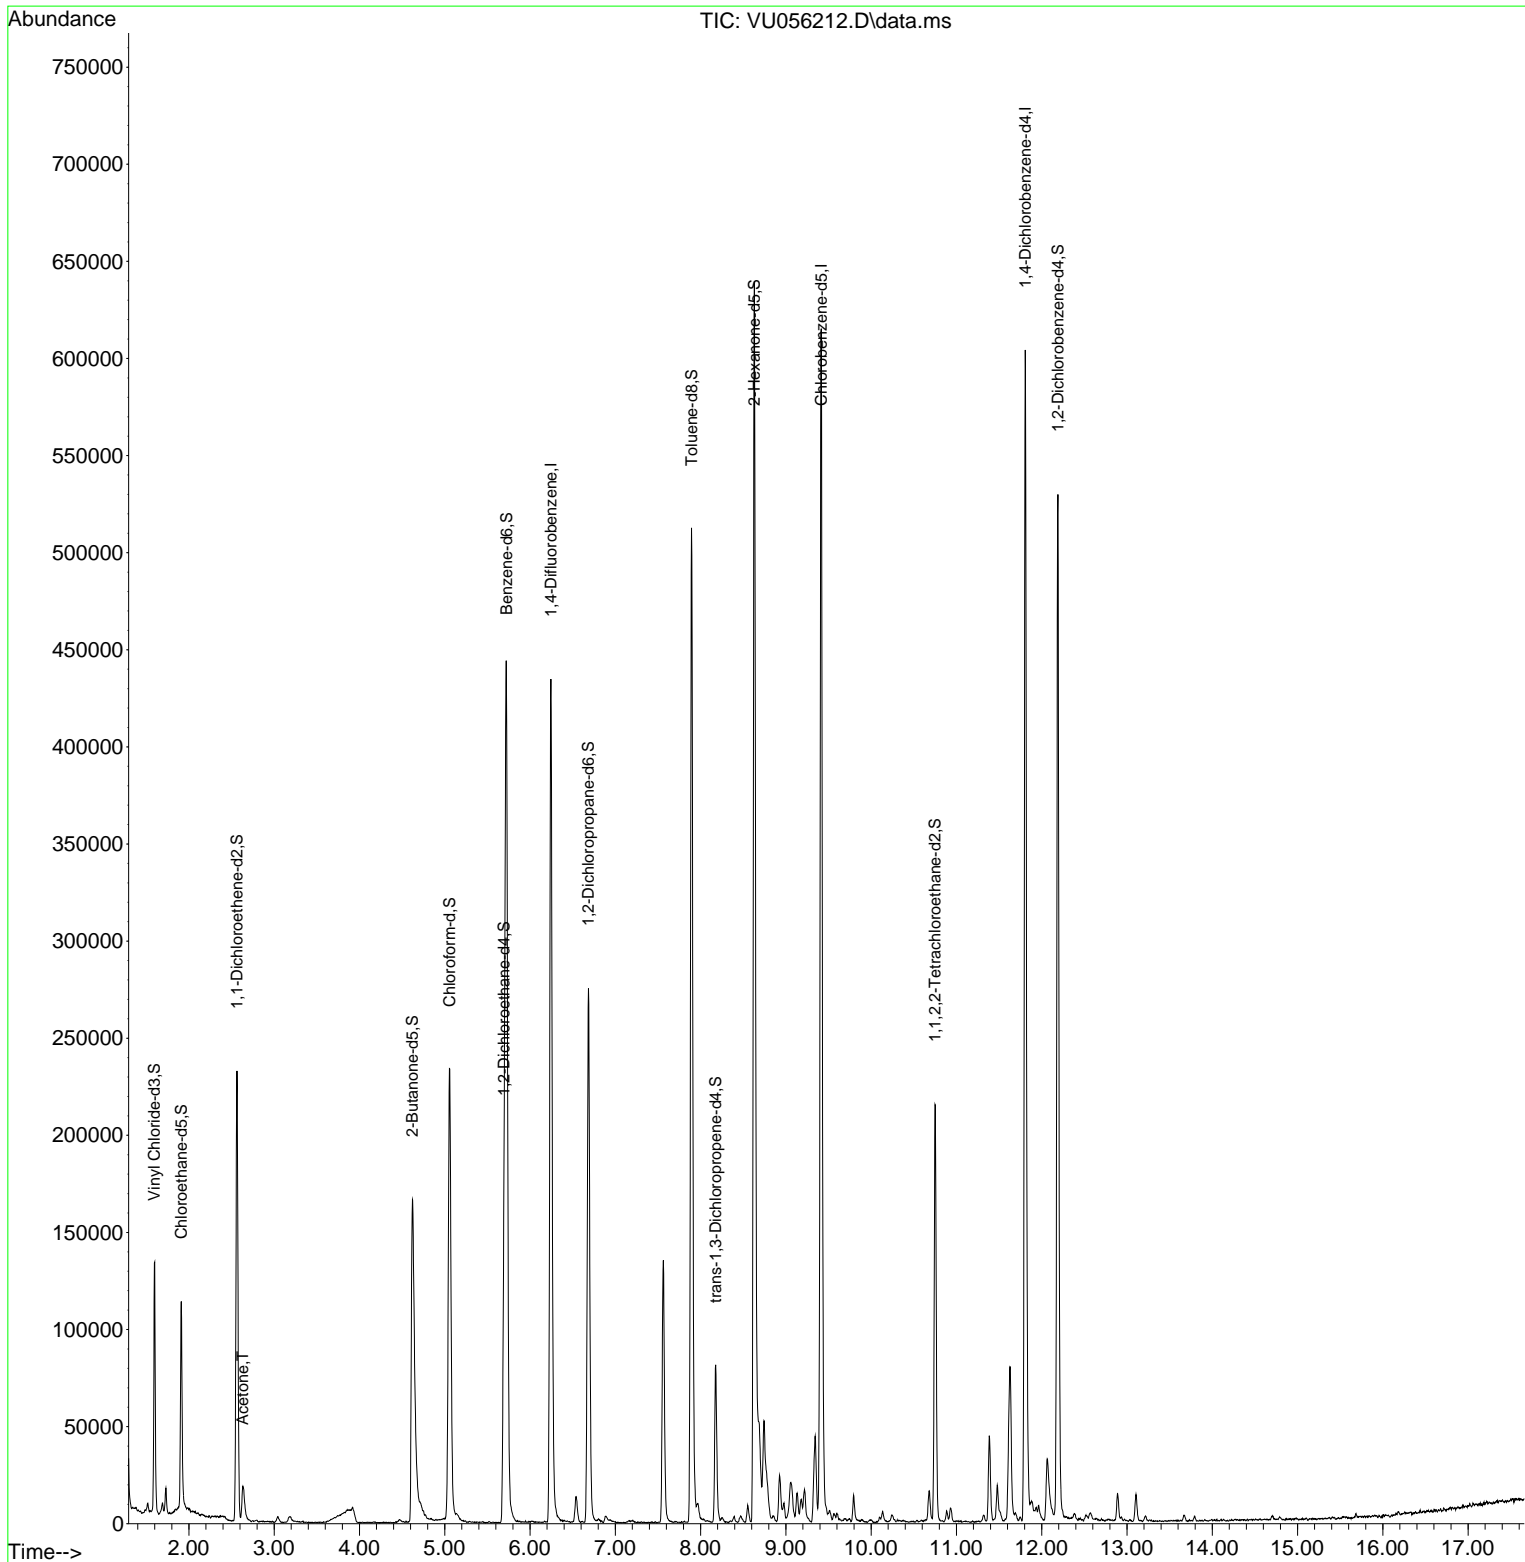

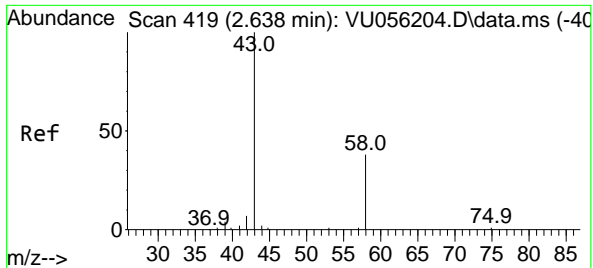

#13  
 Acetone  
 Concen: 9.672 ug/L  
 RT: 2.631 min Scan# 41  
 Delta R.T. -0.007 min  
 Lab File: VU056212.D  
 Acq: 11 Nov 2023 13:13

Instrument : MSVOA\_U  
 ClientSampleId : GCDL1

Tgt Ion: 43 Resp: 27058  
 Ion Ratio Lower Upper  
 43 100  
 58 38.7 0.0 74.4

