

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111123\
 Data File : VU056221.D
 Acq On : 11 Nov 2023 16:52
 Operator : MD/SY
 Sample : 05339-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDK4

Quant Time: Nov 11 20:23:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 11 20:19:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	363331	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	363246	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	167981	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	87290	3.871	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.911	69	83276	5.441	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.800%
11) 1,1-Dichloroethene-d2	2.563	65	43199	4.348	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.000%
20) 2-Butanone-d5	4.637	46	272588	73.677	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	147.360%#
24) Chloroform-d	5.058	84	218647	5.093	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	5.695	65	104354	5.521	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.721	84	434274	4.978	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	6.685	67	137579	5.357	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%
41) Toluene-d8	7.894	98	362678	4.537	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	8.177	79	47871	4.877	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.600%
46) 2-Hexanone-d5	8.631	63	224296	69.712	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	139.420%#
56) 1,1,2,2-Tetrachloroeth...	10.753	84	109476	5.973	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	119.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	140607	5.428	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds					Qvalue	
13) Acetone	2.653	43	23831	8.734	ug/L	75
34) Trichloroethene	6.541	95	17504	0.616	ug/L	93
47) Tetrachloroethene	8.550	164	7173	0.336	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111123\
Data File : VU056221.D
Acq On : 11 Nov 2023 16:52
Operator : MD/SY
Sample : 05339-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDK4

Quant Time: Nov 11 20:23:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 11 20:19:10 2023
Response via : Initial Calibration

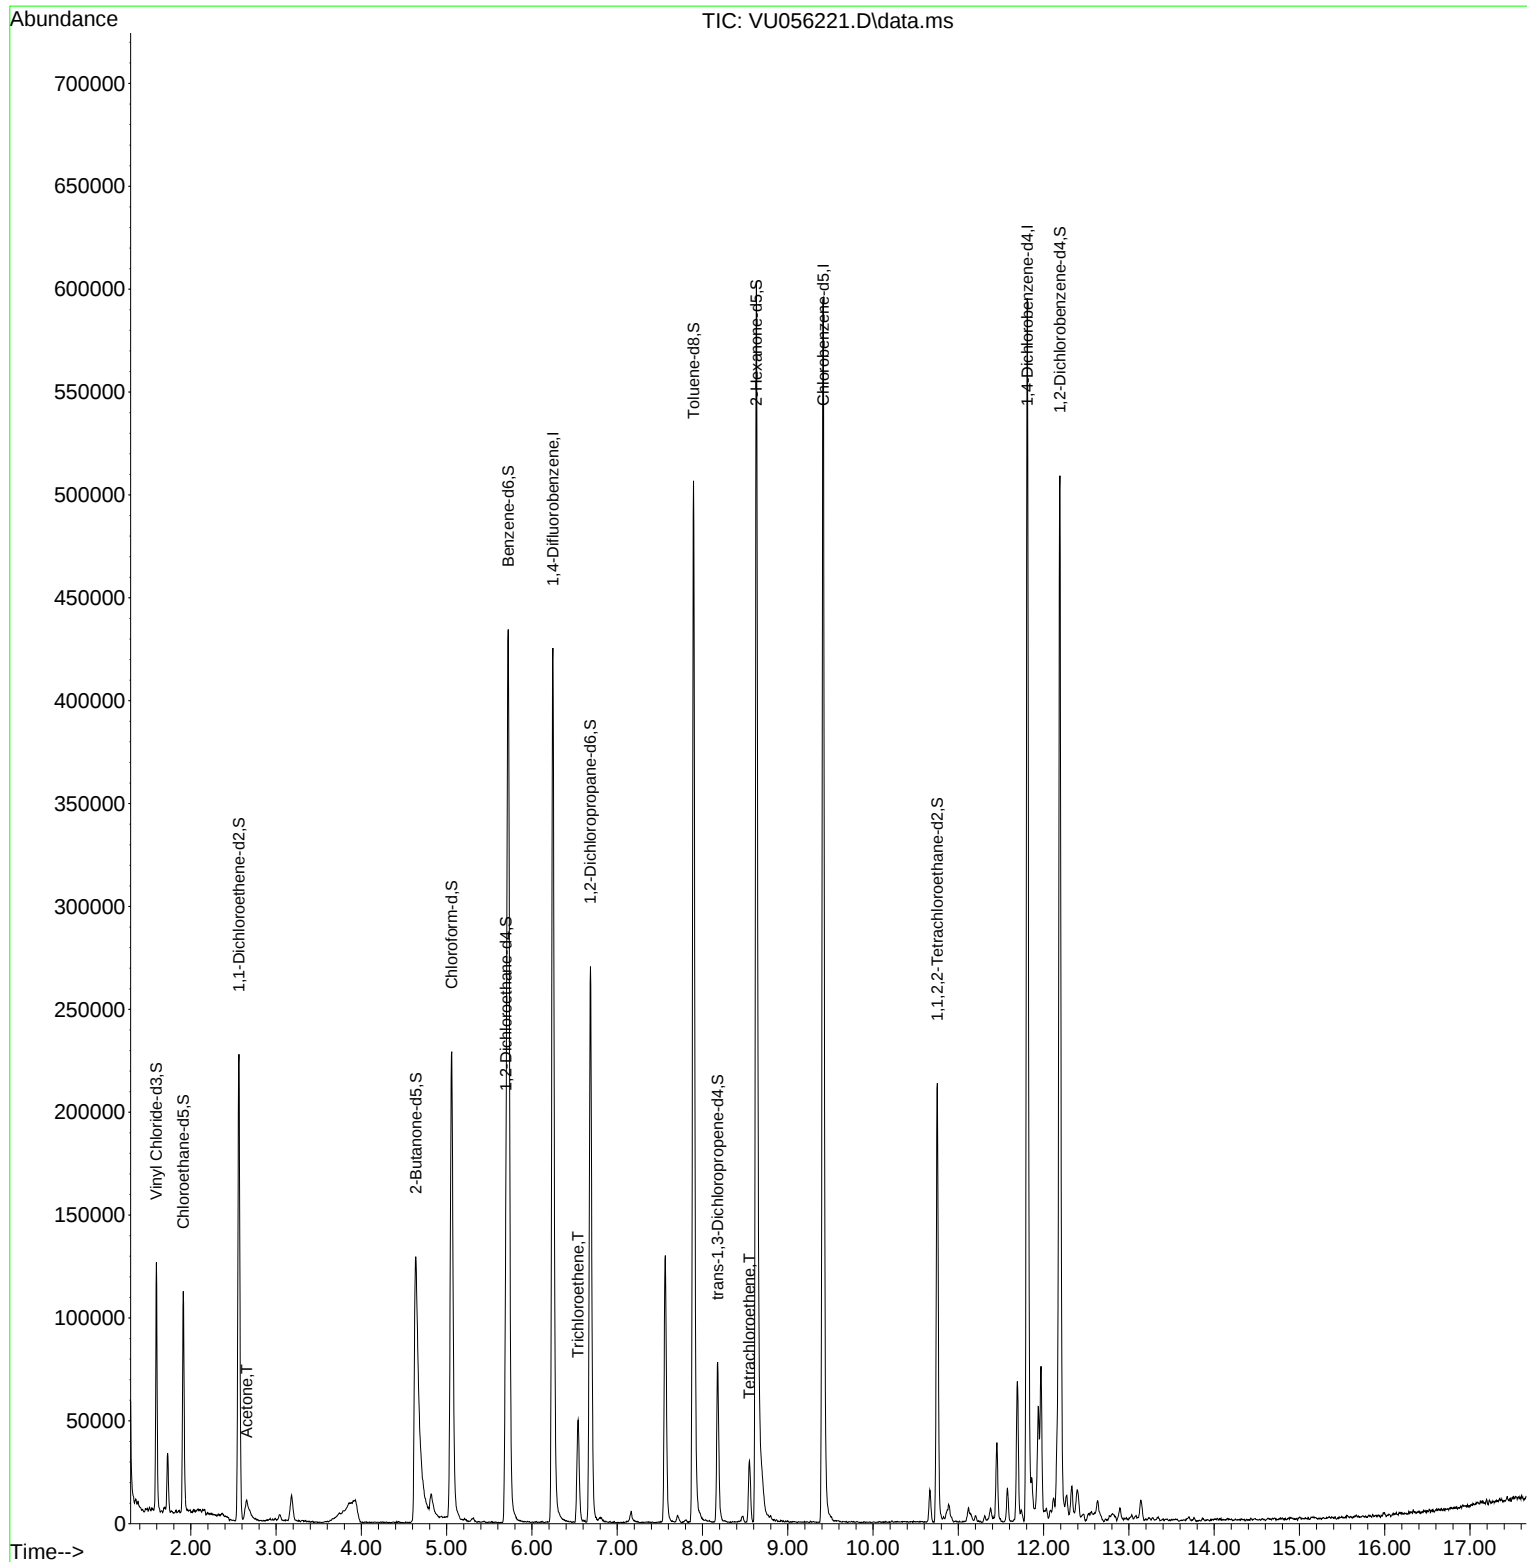

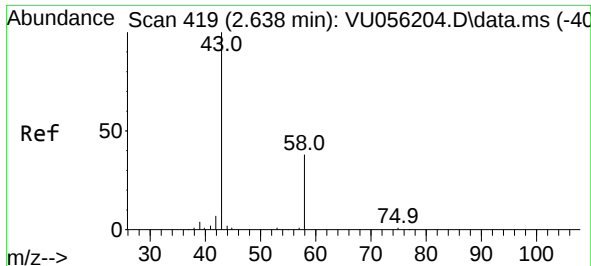

#13

Acetone

Concen: 8.734 ug/L

RT: 2.653 min Scan# 419

Delta R.T. 0.016 min

Lab File: VU056221.D

Acq: 11 Nov 2023 16:52

Instrument :

MSVOA_U

ClientSampleId :





GCDK4

Tgt Ion: 43 Resp: 23831

Ion Ratio Lower Upper

43 100

58 22.3 0.0 74.4

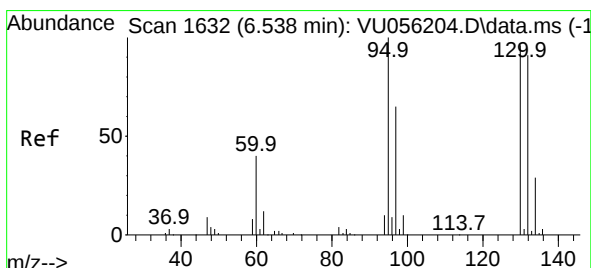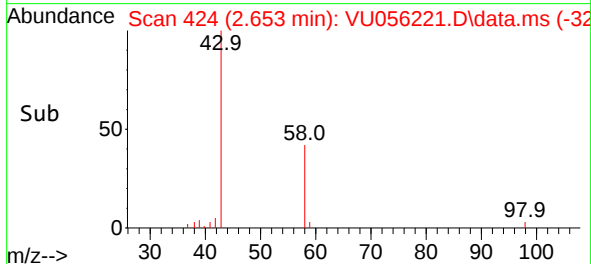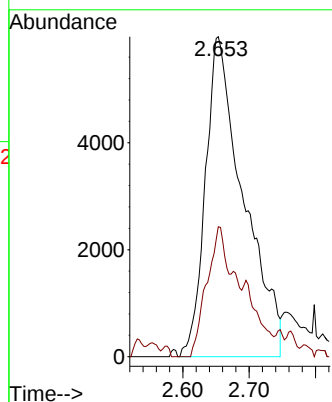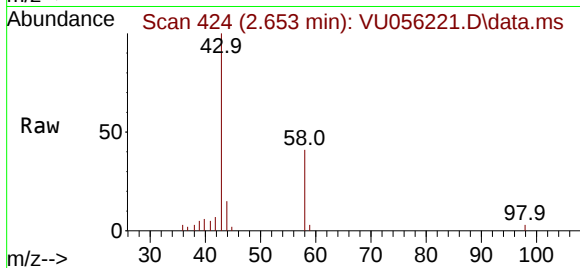

#34

Trichloroethene

Concen: 0.616 ug/L

RT: 6.541 min Scan# 1633

Delta R.T. 0.003 min

Lab File: VU056221.D

Acq: 11 Nov 2023 16:52

Tgt Ion: 95 Resp: 17504




Ion Ratio Lower Upper


95 100

97 55.7 46.8 87.0

132 93.4 66.5 123.5


130 93.5 70.6 131.0

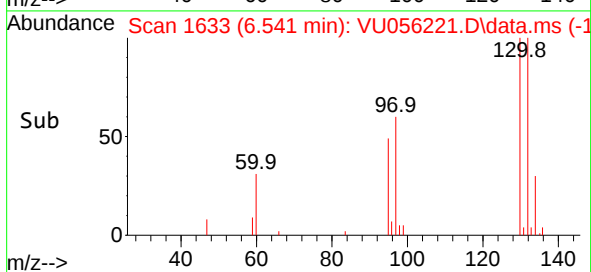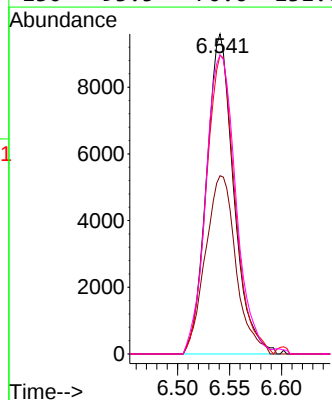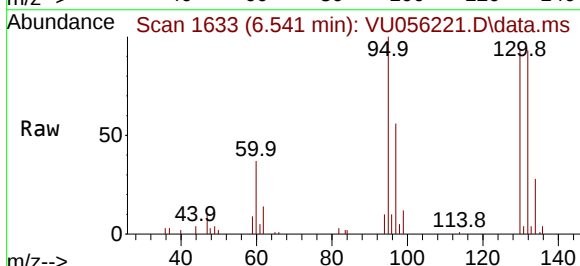

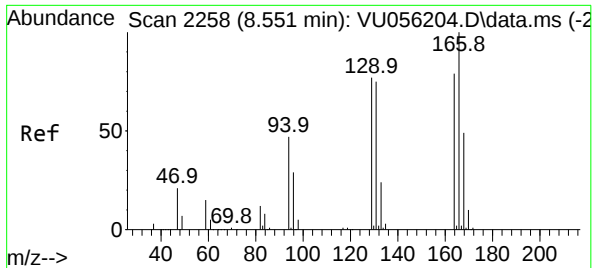

#47
 Tetrachloroethene
 Concen: 0.336 ug/L
 RT: 8.550 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VU056221.D
 Acq: 11 Nov 2023 16:52

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDK4

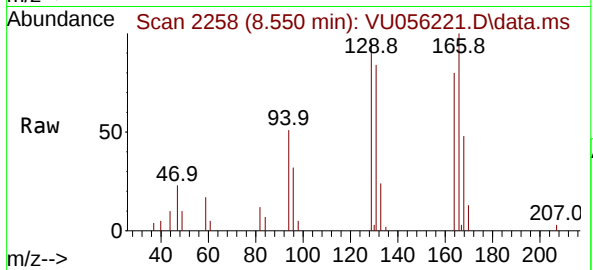

Tgt Ion:	164	Resp:	7173
Ion	Ratio	Lower	Upper
164	100		
129	120.3	66.6	123.8
131	104.7	67.8	126.0
166	125.4	85.9	159.5

