


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111123\
Data File : VU056203.D
Acq On : 11 Nov 2023 08:52
Operator : MD/SY
Sample : BFB071
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB071

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 11 22:15:12 2023

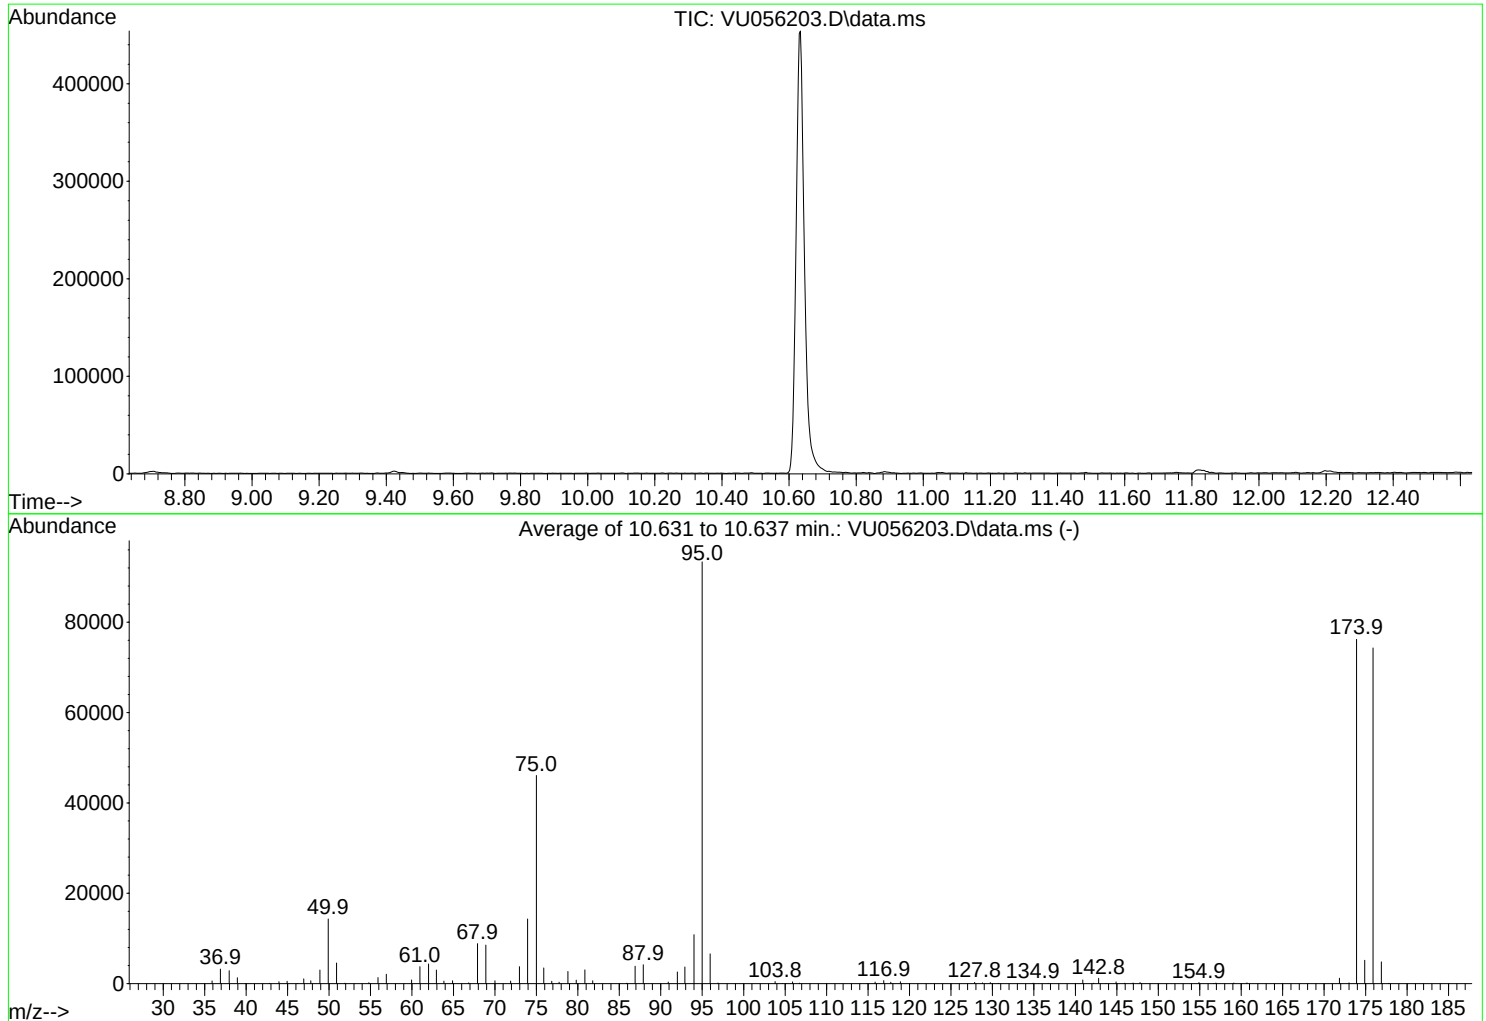

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	14308	PASS
75	95	30	80	49.4	46085	PASS
95	95	100	100	100.0	93357	PASS
96	95	5	9	7.1	6582	PASS
173	174	0.00	2	0.2	188	PASS
174	95	50	120	81.7	76229	PASS
175	174	5	9	6.8	5171	PASS
176	174	95	101	97.5	74307	PASS
177	176	5	9	6.5	4814	PASS

Scan 2891 (10.586 min): VU056203.D\data.ms
BFB071

m/z	Abundance
39.90	234.0
43.90	548.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
36.00	615.0
36.90	3442.0
38.00	3002.0
38.90	1353.0
40.10	253.0
44.00	977.0
45.00	519.0
46.20	143.0
47.00	958.0
47.80	810.0
48.90	3194.0
49.90	14910.0
50.90	4459.0
51.90	161.0
54.80	268.0
55.90	1313.0
56.90	2112.0
60.00	861.0
60.90	3855.0
62.00	4698.0
63.00	3247.0
63.90	570.0
64.90	674.0
66.90	213.0
67.90	9619.0
68.90	8753.0
70.00	750.0
71.90	599.0
72.90	3959.0
74.00	15338.0
75.00	47040.0
75.90	3774.0
76.80	507.0
77.90	301.0
78.80	2716.0
79.80	806.0
80.90	3188.0
81.80	606.0
85.90	132.0
86.90	4160.0
87.90	4221.0
90.90	365.0
92.00	2626.0
92.90	3796.0
94.00	11340.0
95.00	95504.0
96.00	6620.0
96.90	135.0
103.80	467.0
104.70	113.0
105.90	397.0
106.80	123.0
115.80	356.0
116.90	725.0
117.70	297.0
118.90	461.0
127.80	352.0
128.80	194.0
129.80	297.0
130.70	199.0
136.70	134.0
140.90	885.0
142.20	183.0
142.80	1136.0
144.90	296.0
146.00	162.0
146.90	177.0
147.80	299.0
155.00	225.0
157.00	230.0
159.10	153.0
160.70	168.0
171.80	1071.0
173.90	76736.0
174.90	5183.0
175.90	75864.0
176.90	4989.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	664.0
36.90	3325.0
37.90	2897.0
39.00	1393.0
40.10	274.0
42.80	119.0
44.00	961.0
44.90	533.0
46.90	1111.0
47.80	687.0
48.90	3076.0
49.90	14829.0
50.90	4719.0
51.90	141.0
54.80	212.0
55.90	1469.0
56.90	2141.0
60.00	828.0
60.90	3921.0
62.00	4506.0
63.00	3069.0
63.80	592.0
64.90	691.0
66.80	192.0
67.90	9073.0
68.90	8721.0
70.00	671.0
71.90	604.0
73.00	3850.0
74.00	14563.0
75.00	47584.0
75.90	3543.0
76.80	558.0
77.70	331.0
78.80	2790.0
79.80	780.0
80.80	3107.0
81.80	640.0
85.90	144.0
86.90	3871.0
87.90	4414.0
90.90	367.0
92.00	2683.0
92.90	3780.0
94.00	11373.0
95.00	96184.0
96.00	6784.0
96.90	138.0
103.80	440.0
105.90	376.0
106.70	125.0
114.90	103.0
115.90	362.0
116.90	694.0
117.70	319.0
118.90	422.0
127.80	321.0
128.80	173.0
129.80	255.0
134.90	147.0
136.70	110.0
140.90	842.0
142.20	128.0
142.80	1199.0
143.70	105.0
144.90	396.0
145.90	133.0
147.00	172.0
147.80	231.0
154.90	267.0
156.90	209.0
159.10	150.0
160.70	214.0
171.80	1255.0
173.90	78624.0
174.90	5480.0
175.90	76864.0
176.90	4892.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.80	585.0
36.90	2892.0
37.90	2656.0
39.00	1227.0
40.00	241.0
42.80	108.0
44.00	941.0
44.90	576.0
46.90	1126.0
47.90	448.0
48.90	2806.0
49.90	13186.0
50.90	4500.0
54.80	121.0
55.90	1305.0
56.90	1977.0
59.90	754.0
61.00	3517.0
62.00	3843.0
62.90	2689.0
63.80	539.0
64.90	602.0
66.80	142.0
67.90	7909.0
68.90	8109.0
70.00	550.0
71.90	506.0
73.00	3499.0
73.90	13033.0
75.00	43632.0
75.90	3132.0
76.90	531.0
77.70	384.0
78.80	2526.0
79.80	713.0
80.80	2829.0
81.80	667.0
85.90	103.0
86.90	3501.0
87.90	3893.0
90.90	311.0
92.00	2463.0
92.90	3474.0
94.00	9851.0
95.00	88384.0
95.90	6343.0
96.90	160.0
103.80	441.0
105.10	125.0
105.90	356.0
106.70	113.0
115.90	364.0
116.90	627.0
117.80	322.0
118.90	394.0
127.90	228.0
128.80	140.0
129.70	212.0
134.90	164.0
140.90	715.0
142.80	1179.0
144.90	445.0
147.00	135.0
147.80	192.0
154.80	258.0
156.70	144.0
159.10	122.0
160.70	159.0
171.90	1257.0
173.00	563.0
173.90	73328.0
174.90	4850.0
175.90	70192.0
176.90	4560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071