

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061602.D
Acq On : 12 Nov 2024 13:15
Operator : MD/SY
Sample : VU1112WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Time: Nov 13 05:07:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Nov 13 05:00:10 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	46549	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	13886	0.860	ug/l	0.00
Spiked Amount	1.000		Recovery	=	86.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	14521	0.903	ug/l	0.00
Spiked Amount	1.000		Recovery	=	90.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061602.D
Acq On : 12 Nov 2024 13:15
Operator : MD/SY
Sample : VU1112WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Time: Nov 13 05:07:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Nov 13 05:00:10 2024
Response via : Initial Calibration




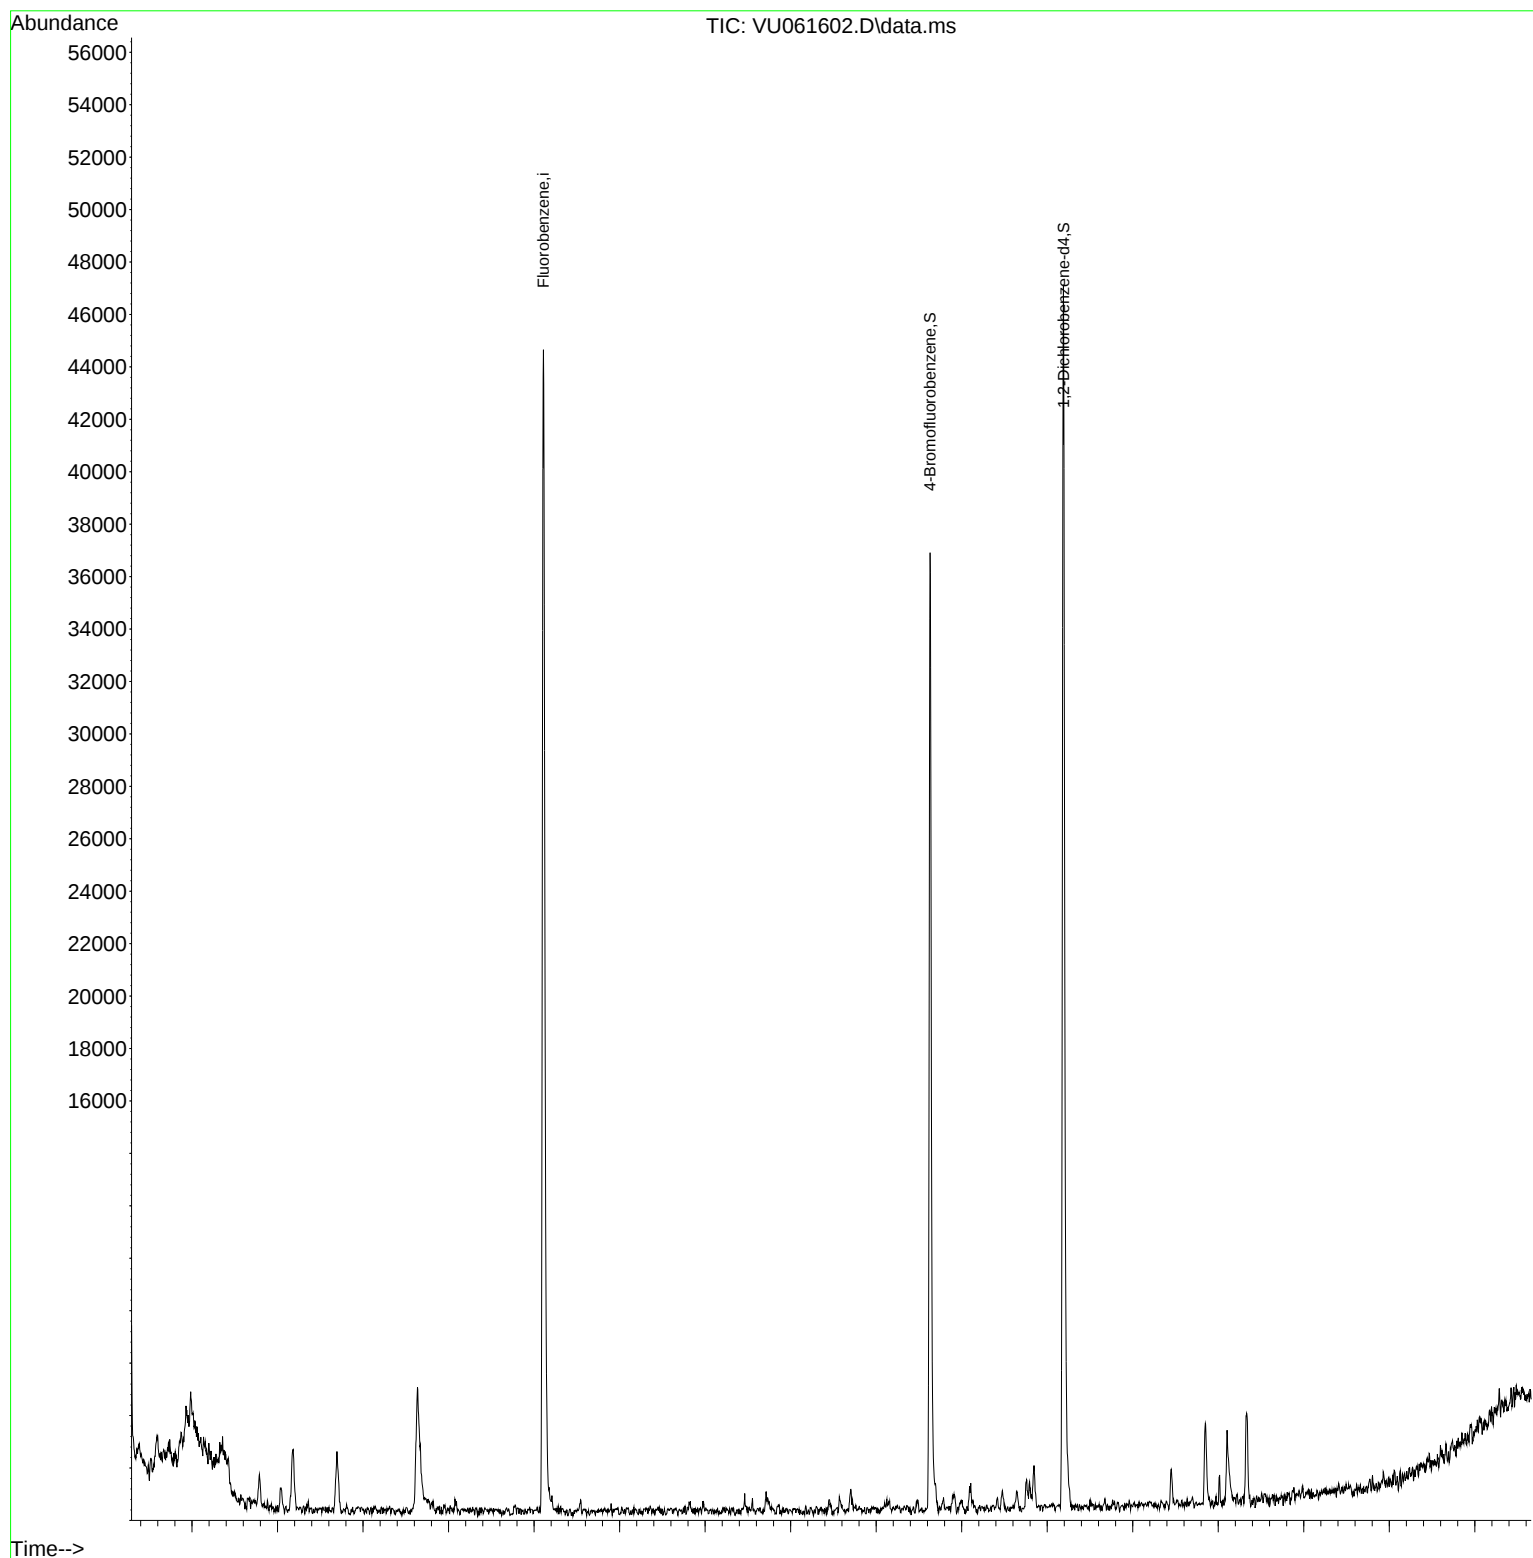


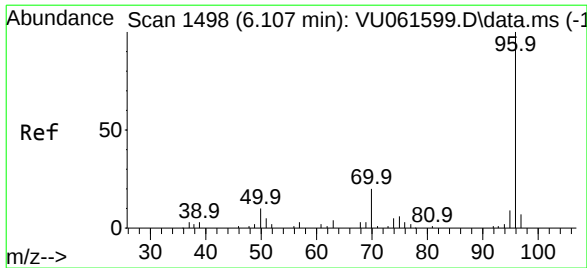

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1498
Delta R.T. 0.003 min
Lab File: VU061602.D
Acq: 12 Nov 2024 13:15




Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01


Tgt Ion:	96	Resp:	46549
Ion	Ratio	Lower	Upper
96	100		
70	19.3	15.8	23.6
95	8.7	7.3	10.9
97	6.7	0.0	0.0

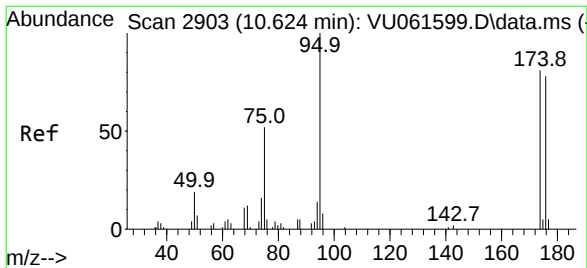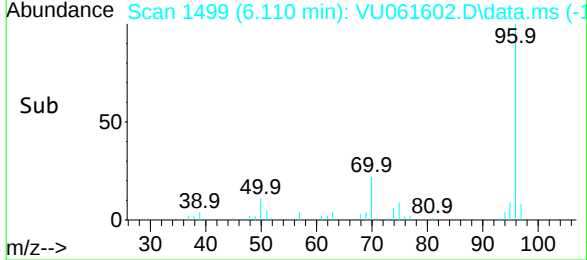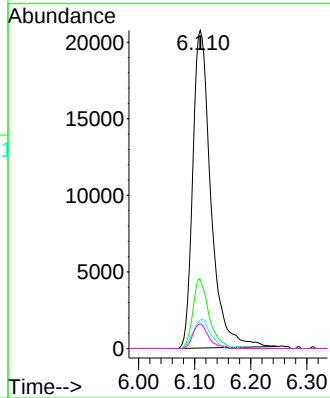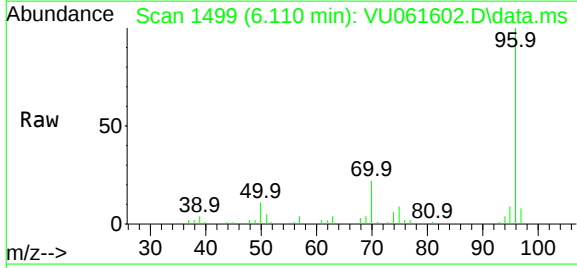

#57
4-Bromofluorobenzene
Concen: 0.860 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.006 min
Lab File: VU061602.D
Acq: 12 Nov 2024 13:15


Tgt Ion:	95	Resp:	13886
Ion	Ratio	Lower	Upper
95	100		
174	82.9	67.5	101.3
176	77.3	62.7	94.1

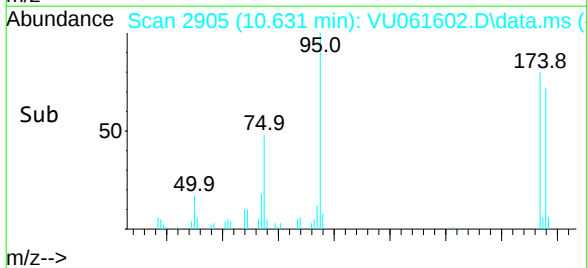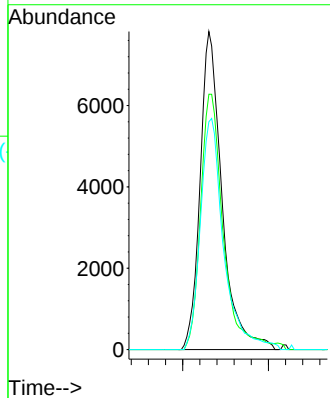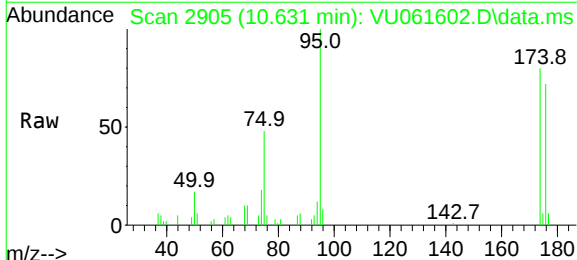

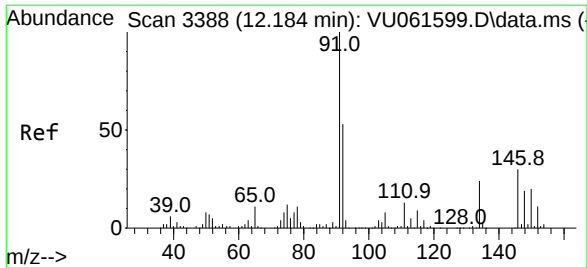

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.903 ug/l
 RT: 12.190 min Scan# 33
 Delta R.T. 0.006 min
 Lab File: VU061602.D
 Acq: 12 Nov 2024 13:15

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1112WBL01

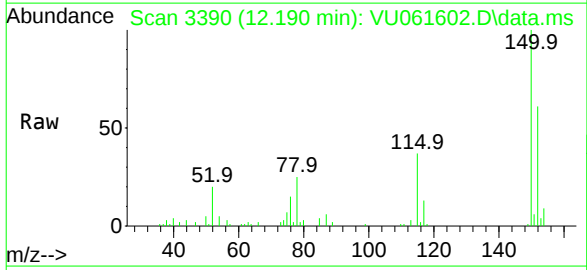

Tgt Ion:	152	Resp:	14521
Ion Ratio	Lower	Upper	
152	100		
115	63.6	0.0	259.0
150	158.9	0.0	650.2

