

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
 Data File : VU061604.D
 Acq On : 12 Nov 2024 15:19
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Nov 13 05:07:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Nov 13 05:00:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	41728	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	13091	0.904	ug/l	0.00
Spiked Amount	1.000		Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	13293	0.922	ug/l	0.00
Spiked Amount	1.000		Recovery	=	92.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061604.D
Acq On : 12 Nov 2024 15:19
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Quant Time: Nov 13 05:07:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Nov 13 05:00:10 2024
Response via : Initial Calibration

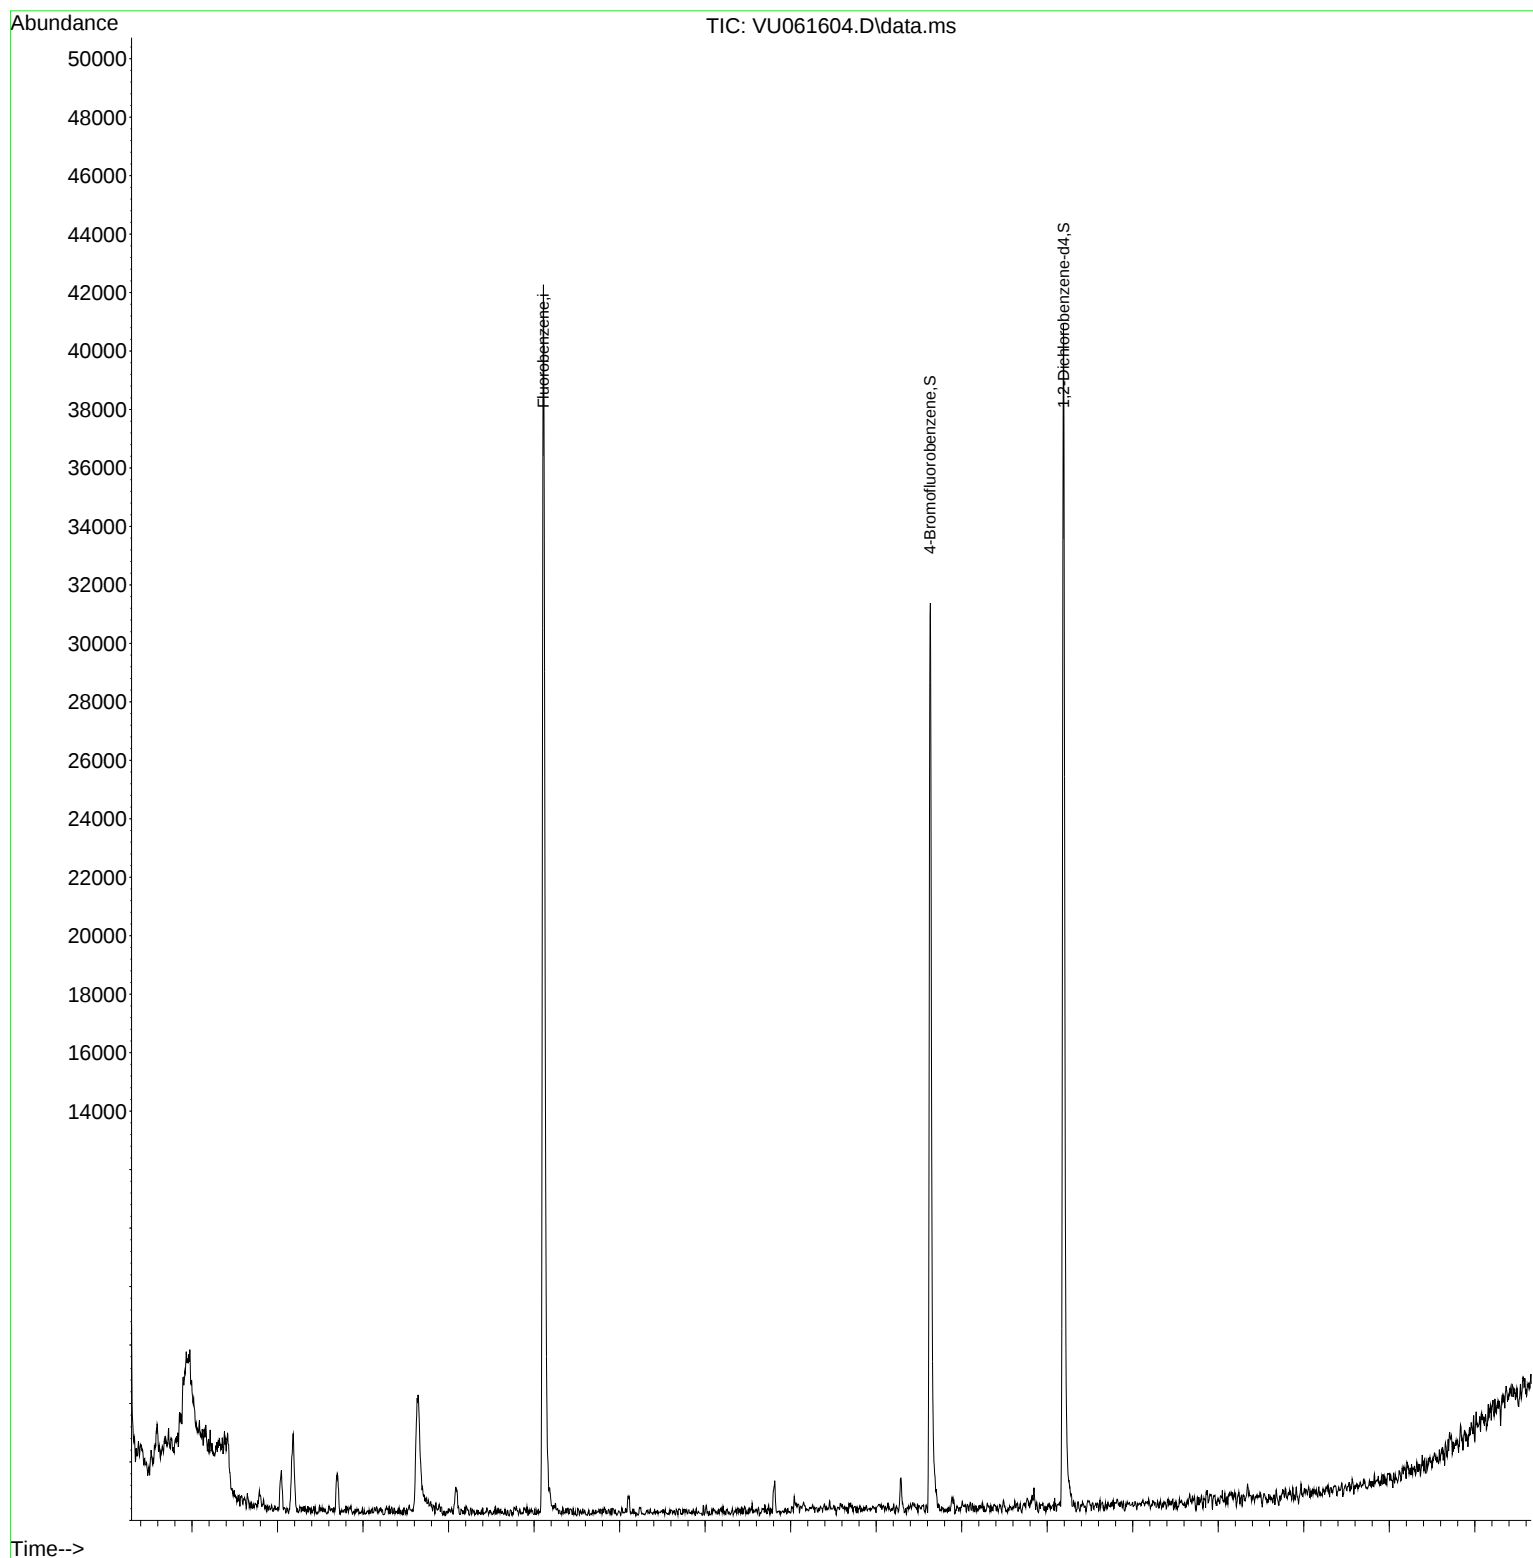



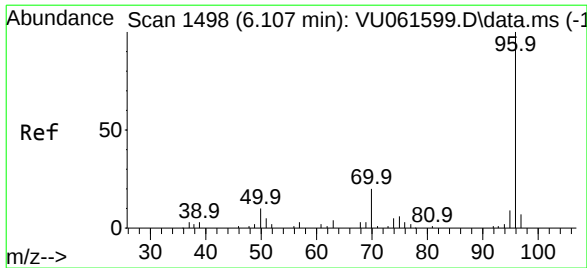


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1498
Delta R.T. 0.003 min
Lab File: VU061604.D
Acq: 12 Nov 2024 15:19


Instrument :
MSVOA_U
ClientSampleId :
VIBLK

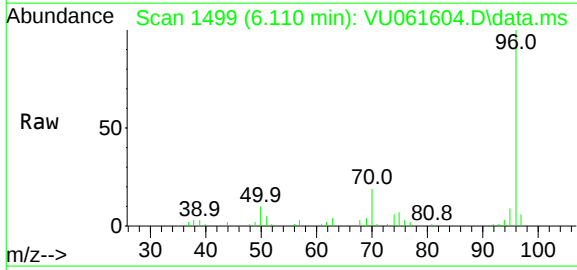



Tgt Ion: 96 Resp: 41728
Ion Ratio Lower Upper
96 100
70 17.7 15.8 23.6
95 9.7 7.3 10.9
97 6.7 0.0 0.0#

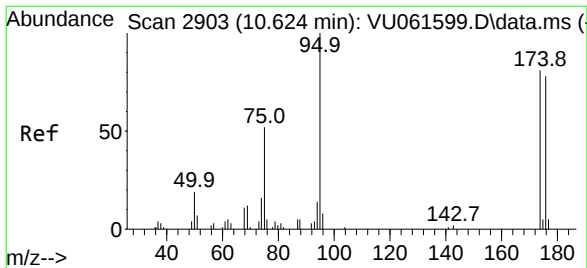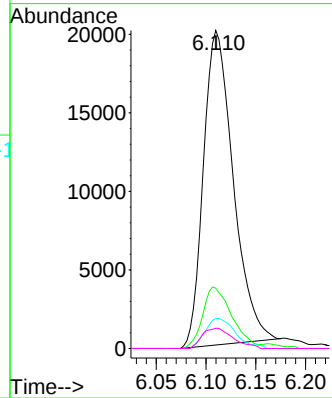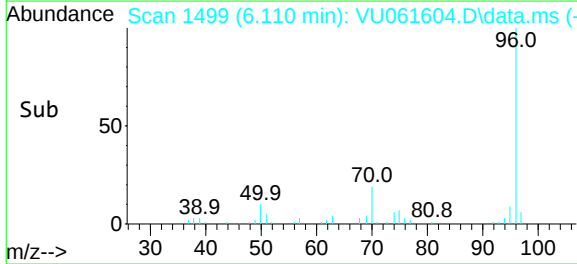


#57
4-Bromofluorobenzene
Concen: 0.904 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.006 min
Lab File: VU061604.D
Acq: 12 Nov 2024 15:19

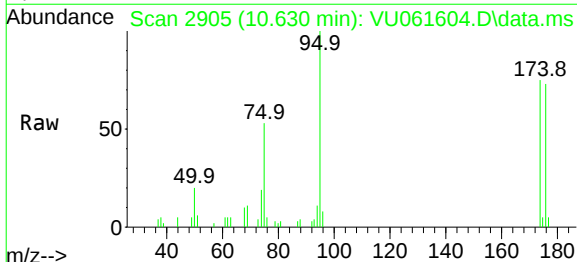


Tgt Ion: 95 Resp: 13091
Ion Ratio Lower Upper
95 100
174 78.5 67.5 101.3
176 74.1 62.7 94.1

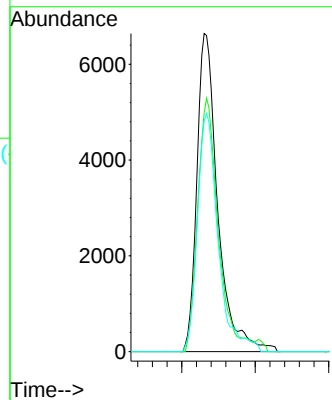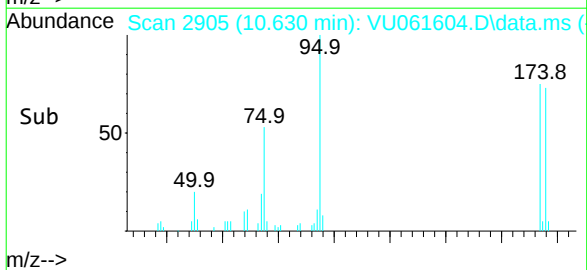

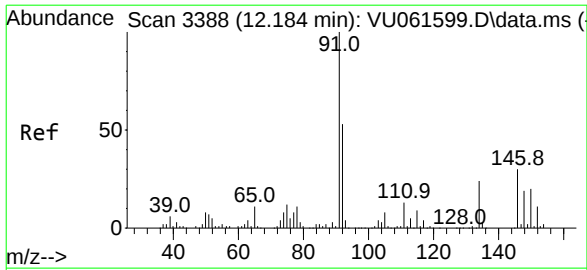

#68
1,2-Dichlorobenzene-d4
Concen: 0.922 ug/l
RT: 12.193 min Scan# 33
Delta R.T. 0.009 min
Lab File: VU061604.D
Acq: 12 Nov 2024 15:19

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

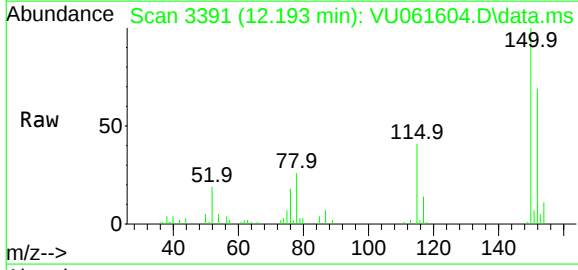

Tgt	Ion:152	Resp:	13293
Ion	Ratio	Lower	Upper
152	100		
115	62.3	0.0	259.0
150	155.4	0.0	650.2

