

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
 Data File : VU061602.D
 Acq On : 12 Nov 2024 13:15
 Operator : MD/SY
 Sample : VU1112WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1112WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU061602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.788	457	466	476	rVB4	1217	2059	2.24%	0.674%
2	3.039	536	544	557	rVB4	976	2092	2.27%	0.685%
3	3.184	574	589	600	rBV2	2333	5491	5.96%	1.797%
4	3.695	736	748	758	rBV4	2323	5028	5.46%	1.645%
5	4.637	1025	1041	1064	rBV2	4634	14906	16.18%	4.878%
6	6.110	1487	1499	1518	rBV	44349	92104	100.00%	30.142%
7	9.705	2608	2617	2621	rBV4	848	1238	1.34%	0.405%
8	10.631	2895	2905	2923	rBV2	36438	63079	68.49%	20.643%
9	11.094	3043	3049	3051	rBV	942	961	1.04%	0.314%
10	11.476	3160	3168	3176	rBV4	735	1246	1.35%	0.408%
11	11.759	3250	3256	3263	rBV4	1029	1678	1.82%	0.549%
12	11.794	3263	3267	3272	rVV3	965	1200	1.30%	0.393%
13	11.846	3276	3283	3294	rVB6	1608	2683	2.91%	0.878%
14	12.190	3379	3390	3417	rBV	46671	89469	97.14%	29.280%
15	13.450	3773	3782	3789	rBV2	1541	2545	2.76%	0.833%
16	13.849	3898	3906	3920	rBV5	3097	5806	6.30%	1.900%
17	14.016	3952	3958	3962	rBV3	1130	1054	1.14%	0.345%
18	14.103	3975	3985	4004	rBV3	2825	6289	6.83%	2.058%
19	14.331	4046	4056	4066	rBV7	3458	6639	7.21%	2.173%




Sum of corrected areas: 305567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061602.D
Acq On : 12 Nov 2024 13:15
Operator : MD/SY
Sample : VU1112WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

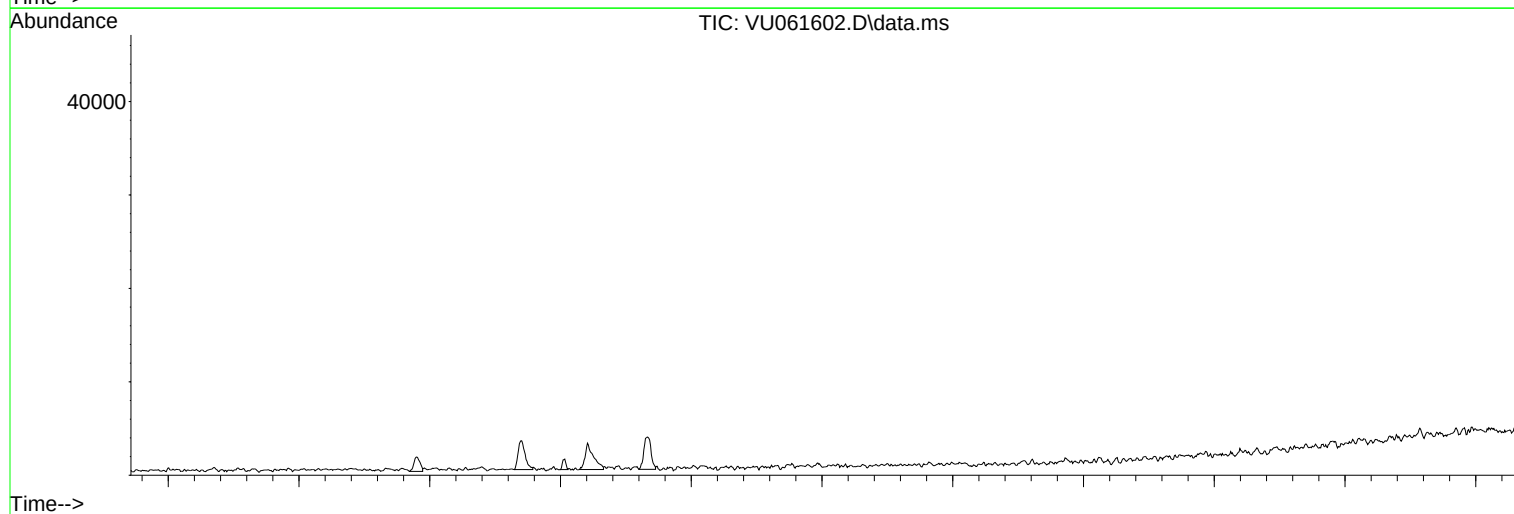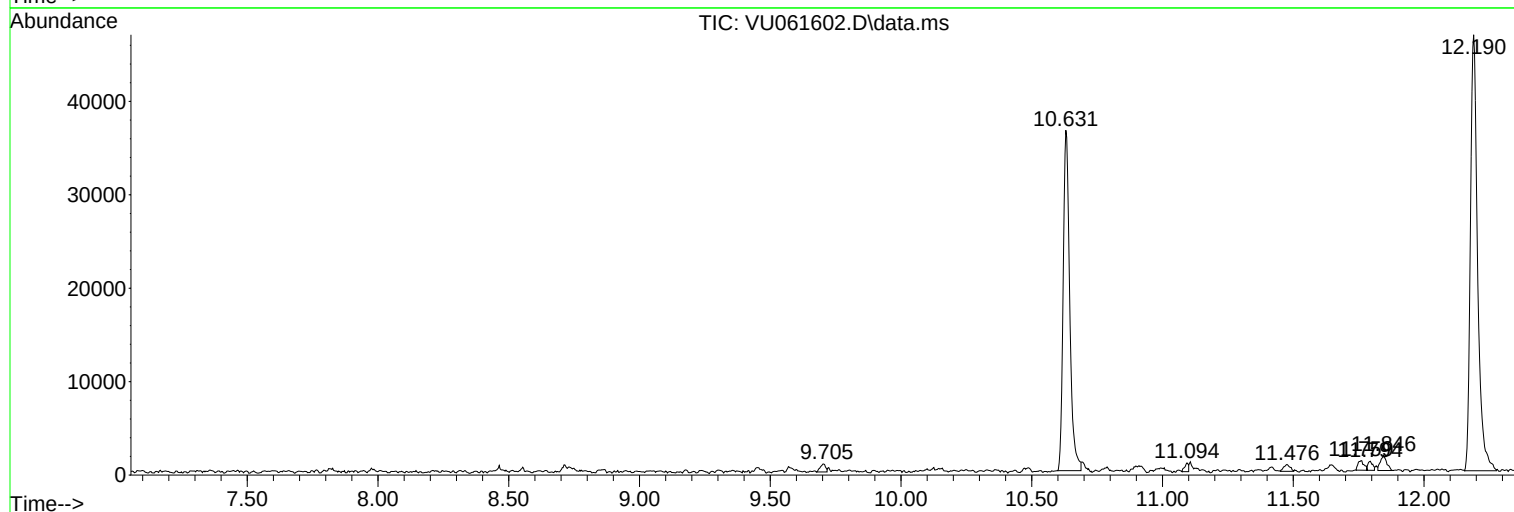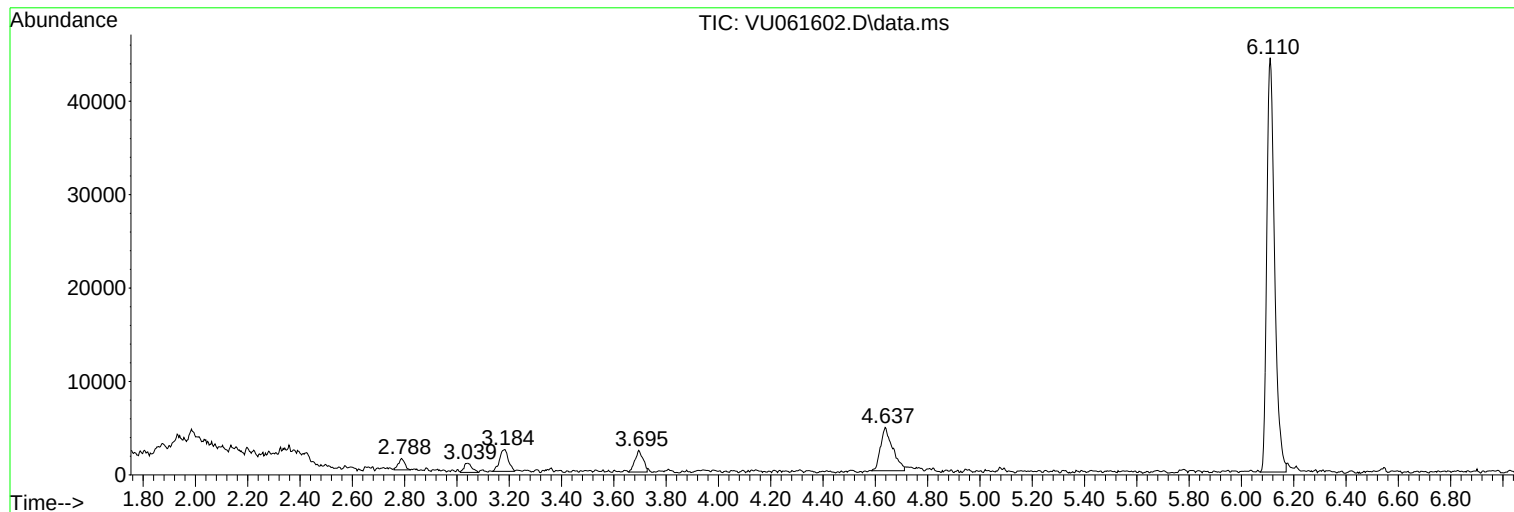

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061602.D
Acq On : 12 Nov 2024 13:15
Operator : MD/SY
Sample : VU1112WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061602.D
Acq On : 12 Nov 2024 13:15
Operator : MD/SY
Sample : VU1112WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------