

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
 Data File : VU061604.D
 Acq On : 12 Nov 2024 15:19
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU061604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.856	172	176	178	rBV2	1103	910	1.05%	0.371%
2	1.895	184	188	191	rBV4	1610	1635	1.88%	0.666%
3	3.046	536	546	554	rBV3	1365	2317	2.67%	0.943%
4	3.184	572	589	603	rBV2	2723	6409	7.39%	2.610%
5	3.695	740	748	749	rBV2	1248	1310	1.51%	0.533%
6	4.634	1024	1040	1041	rBV3	3881	5690	6.56%	2.317%
7	5.084	1171	1180	1183	rBV4	917	1359	1.57%	0.553%
8	6.110	1487	1499	1519	rBV2	41998	86777	100.00%	35.335%
9	8.814	2332	2340	2347	rBV3	1119	1706	1.97%	0.695%
10	10.290	2789	2799	2804	rBV6	1167	1730	1.99%	0.704%
11	10.634	2896	2906	2927	rBV2	31113	58754	67.71%	23.924%
12	12.190	3380	3390	3409	rBV2	40429	74744	86.13%	30.435%
13	17.016	4886	4891	4894	rBV5	1014	1000	1.15%	0.407%
14	17.322	4980	4986	4988	rBV7	1063	1241	1.43%	0.505%




Sum of corrected areas: 245582

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061604.D
Acq On : 12 Nov 2024 15:19
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

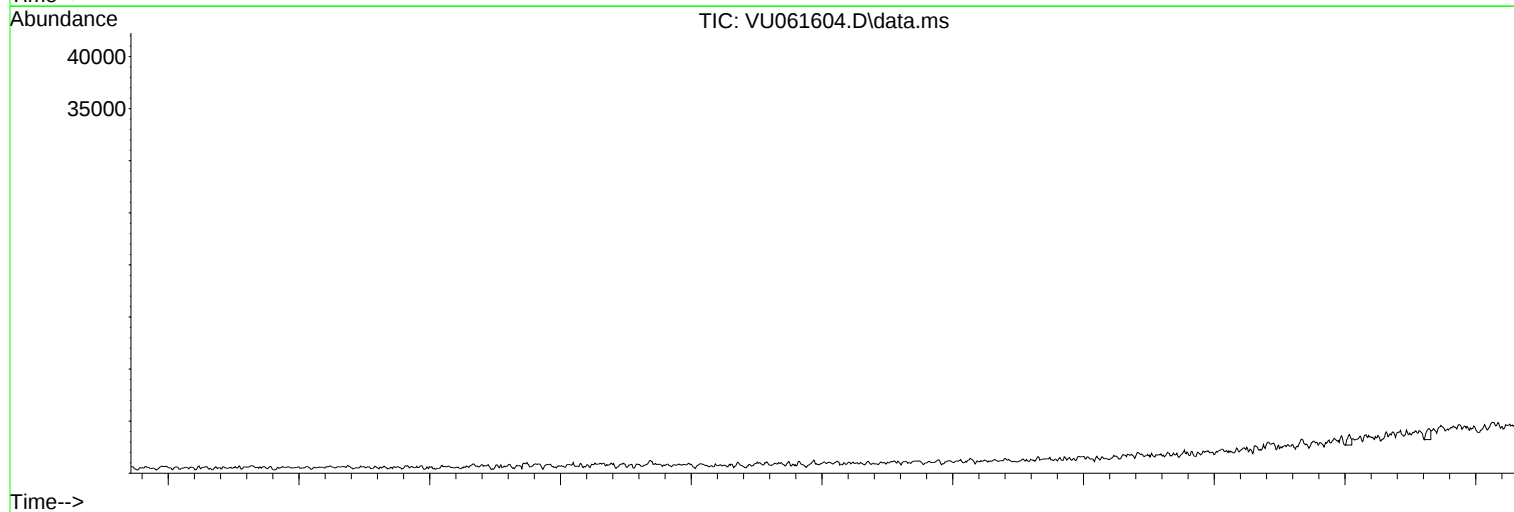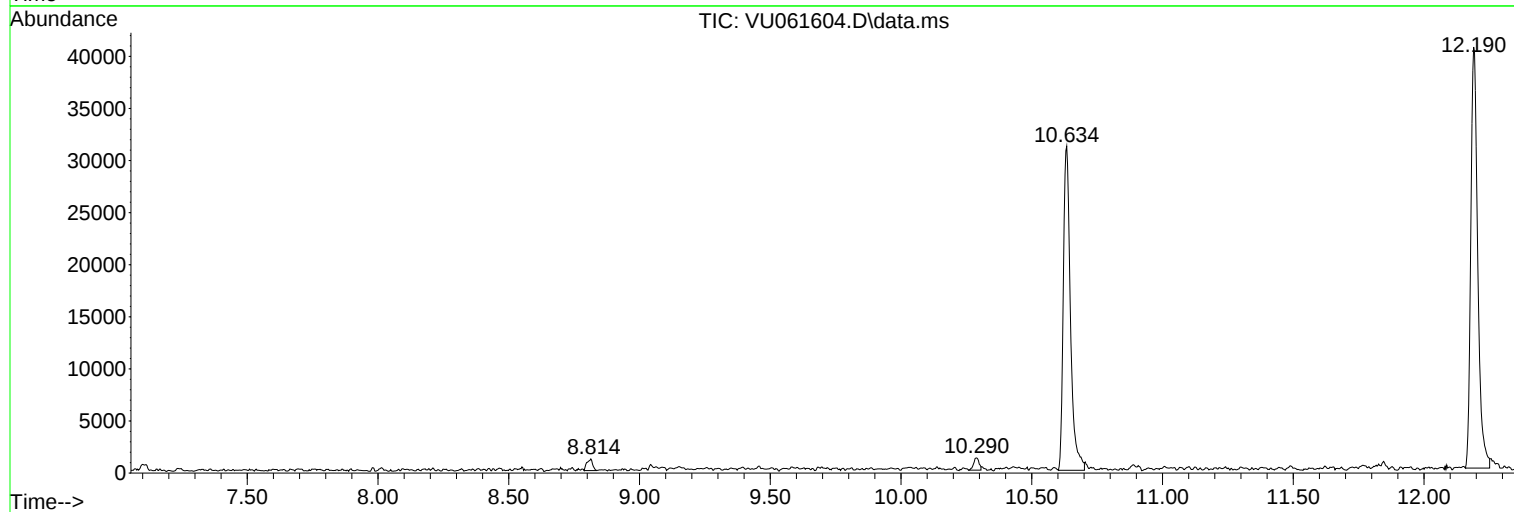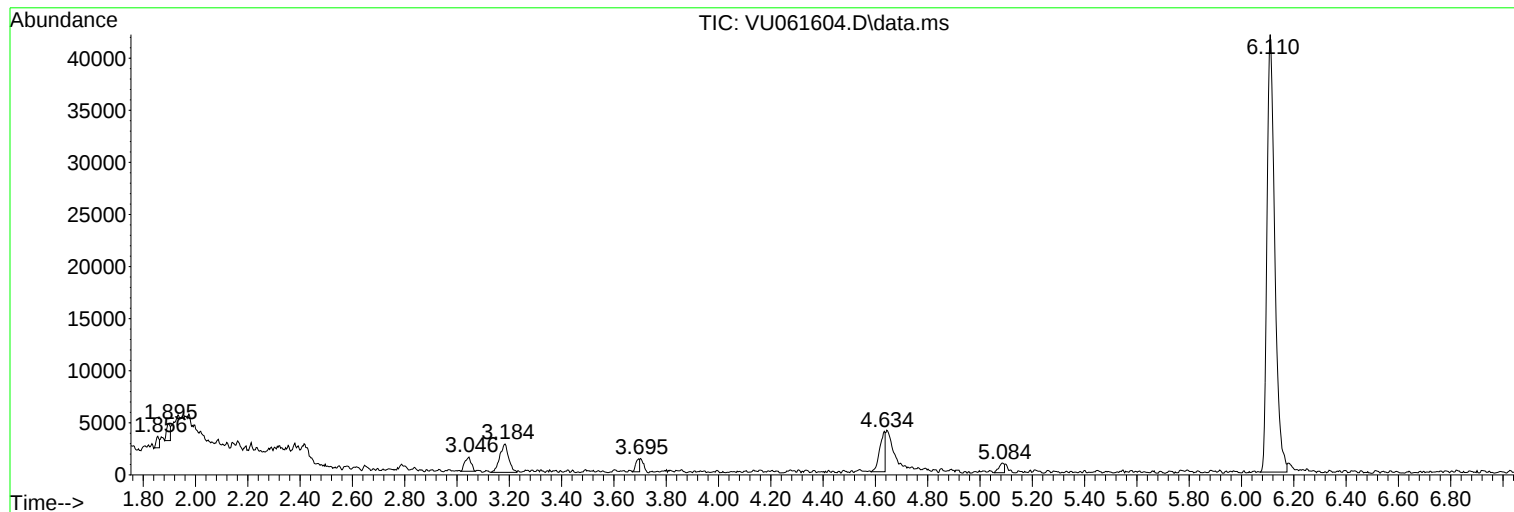

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061604.D
Acq On : 12 Nov 2024 15:19
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061604.D
Acq On : 12 Nov 2024 15:19
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------