
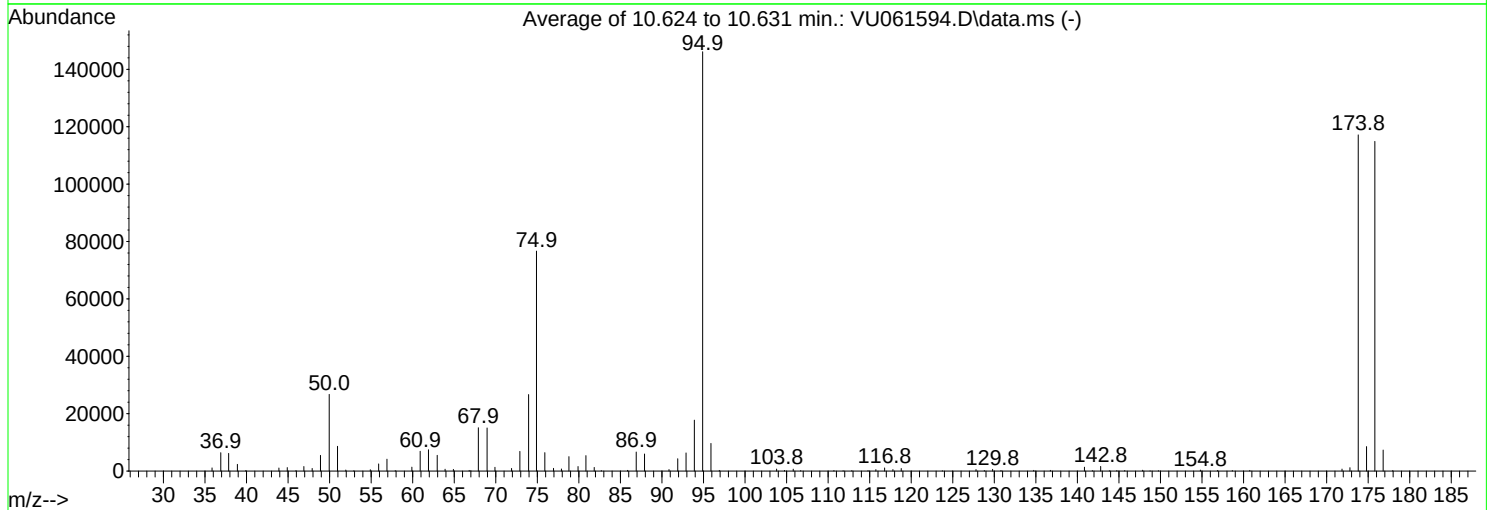


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111224\
Data File : VU061594.D
Acq On : 12 Nov 2024 07:51
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U111224DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Nov 13 05:00:10 2024

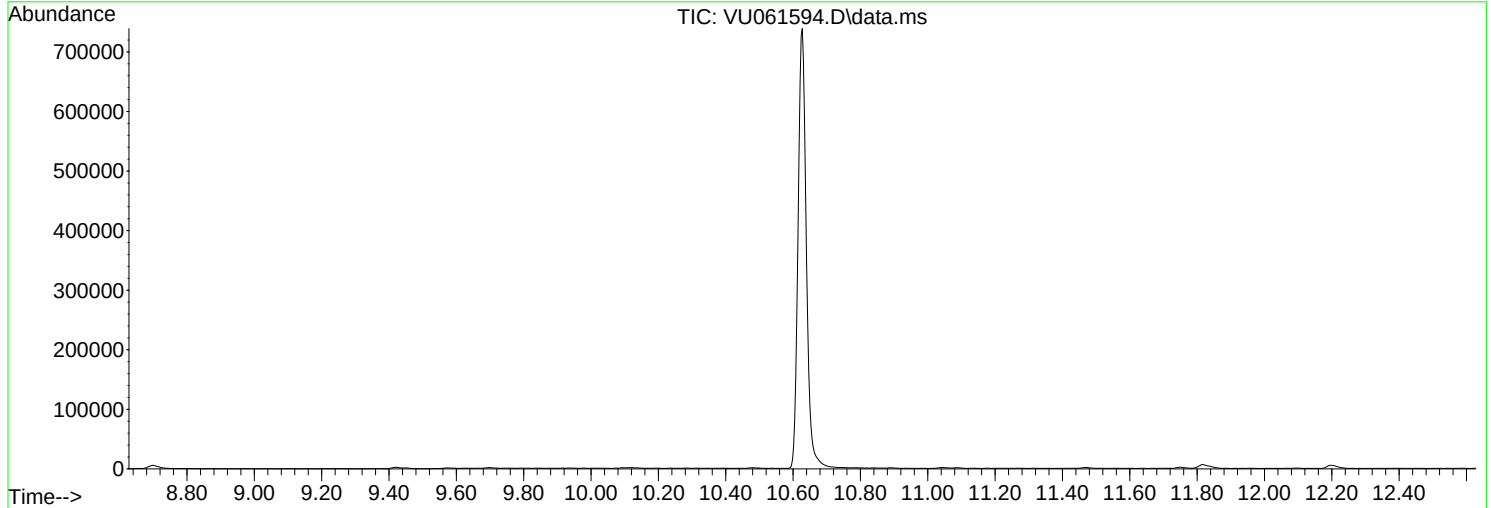

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	26728	PASS
75	95	30	60	52.5	76667	PASS
95	95	100	100	100.0	146133	PASS
96	95	5	9	6.6	9641	PASS
173	174	0.00	2	1.0	1187	PASS
174	95	50	100	80.2	117155	PASS
175	174	5	9	7.3	8540	PASS
176	174	95	101	98.1	114883	PASS
177	176	5	9	6.4	7328	PASS