

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
 Data File : VU061648.D
 Acq On : 14 Nov 2024 01:49
 Operator : MD/SY
 Sample : P4803-14
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AQ9

Quant Time: Nov 14 04:09:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 14 04:06:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	185541	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	173545	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	77052	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	57914	4.831	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.907	69	47006	4.593	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.800%
11) 1,1-Dichloroethene-d2	2.557	65	24420	4.540	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.800%
20) 2-Butanone-d5	4.656	46	102093	40.123	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.240%
24) Chloroform-d	5.052	84	104538	4.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.692	65	54012	4.723	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.717	84	226297	4.713	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
36) 1,2-Dichloropropane-d6	6.679	67	68857	4.863	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.891	98	205095	4.583	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	8.174	79	20820	3.992	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.627	63	92206	44.736	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.480%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	48623	4.356	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	68402	4.984	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds					Qvalue	
25) Chloroform	5.074	83	6405	0.271	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
Data File : VU061648.D
Acq On : 14 Nov 2024 01:49
Operator : MD/SY
Sample : P4803-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AQ9

Quant Time: Nov 14 04:09:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 14 04:06:27 2024
Response via : Initial Calibration

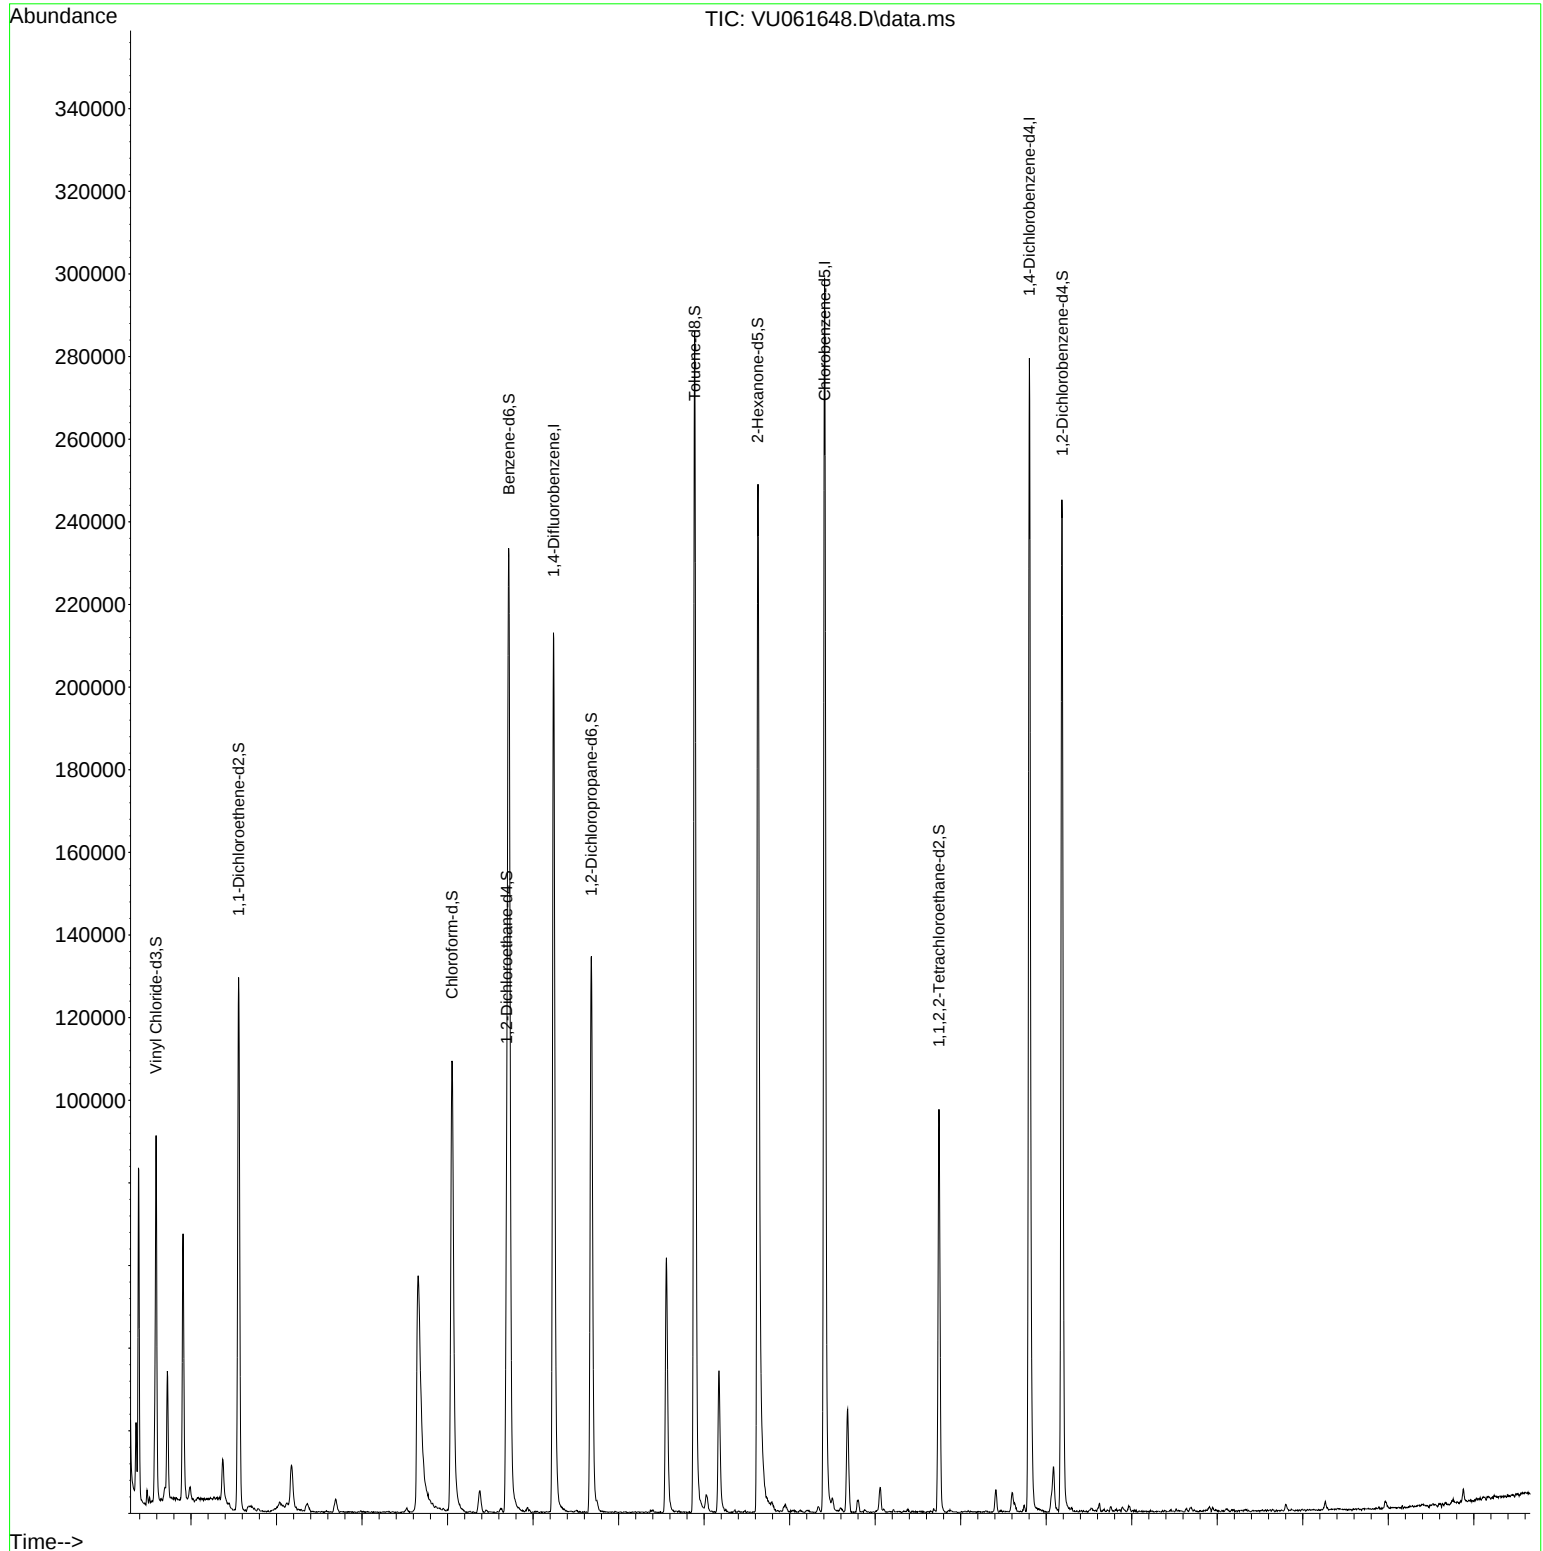

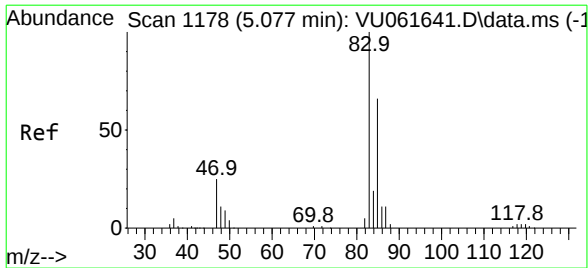

#25
 Chloroform
 Concen: 0.271 ug/L
 RT: 5.074 min Scan# 11
 Delta R.T. -0.003 min
 Lab File: VU061648.D
 Acq: 14 Nov 2024 01:49

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AQ9

Tgt Ion:	83	Resp:	6405
Ion Ratio	Lower	Upper	
83	100		
85	66.0	44.1	81.9

