

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
 Data File : VU061654.D
 Acq On : 14 Nov 2024 04:16
 Operator : MD/SY
 Sample : P4803-18 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AS3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	23	30	42	rVB2	20942	24160	3.33%	0.433%
2	1.595	84	95	108	rBV	74974	97548	13.45%	1.749%
3	1.727	110	136	148	rBV3	19120	84689	11.67%	1.518%
4	1.911	185	193	211	rVB	55470	80823	11.14%	1.449%
5	2.554	382	393	409	rVB	129754	210866	29.07%	3.780%
6	3.174	570	586	602	rBV2	13354	33287	4.59%	0.597%
7	3.685	731	745	766	rBV2	41917	95991	13.23%	1.721%
8	4.650	1024	1045	1080	rBV2	72267	245518	33.84%	4.402%
9	5.055	1153	1171	1202	rBV2	126181	326848	45.06%	5.860%
10	5.714	1356	1376	1389	rBV2	240246	620171	85.49%	11.118%
11	6.238	1527	1539	1563	rBV	213621	417796	57.59%	7.490%
12	6.679	1663	1676	1702	rBV	138180	280609	38.68%	5.031%
13	7.560	1939	1950	1969	rBV	60677	112752	15.54%	2.021%
14	7.891	2040	2053	2069	rBV	273823	494999	68.23%	8.874%
15	7.968	2069	2077	2090	rVB	8189	17785	2.45%	0.319%
16	8.174	2129	2141	2158	rBV	34010	62473	8.61%	1.120%
17	8.643	2274	2287	2321	rBV2	224757	574646	79.21%	10.302%
18	9.409	2510	2525	2563	rBV2	295567	725433	100.00%	13.005%
19	10.753	2929	2943	2959	rBV	103766	177586	24.48%	3.184%
20	11.804	3258	3270	3296	rBV	267672	473189	65.23%	8.483%
21	12.187	3377	3389	3421	rBV	242433	420874	58.02%	7.545%

Sum of corrected areas: 5578043




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
Data File : VU061654.D
Acq On : 14 Nov 2024 04:16
Operator : MD/SY
Sample : P4803-18 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

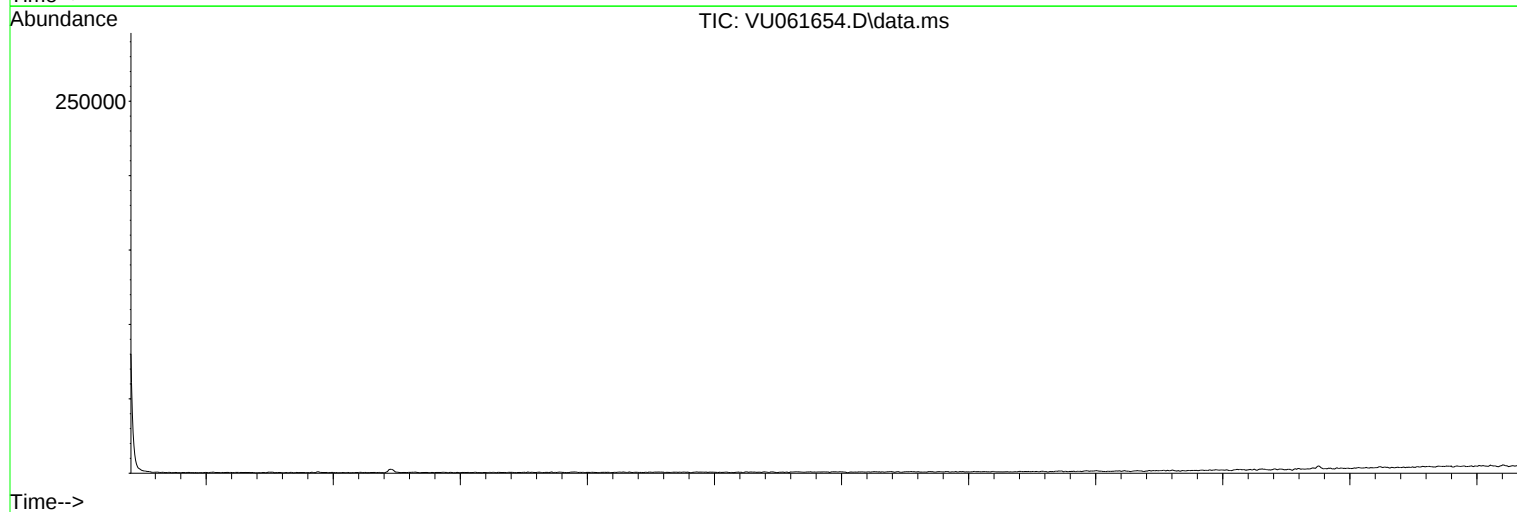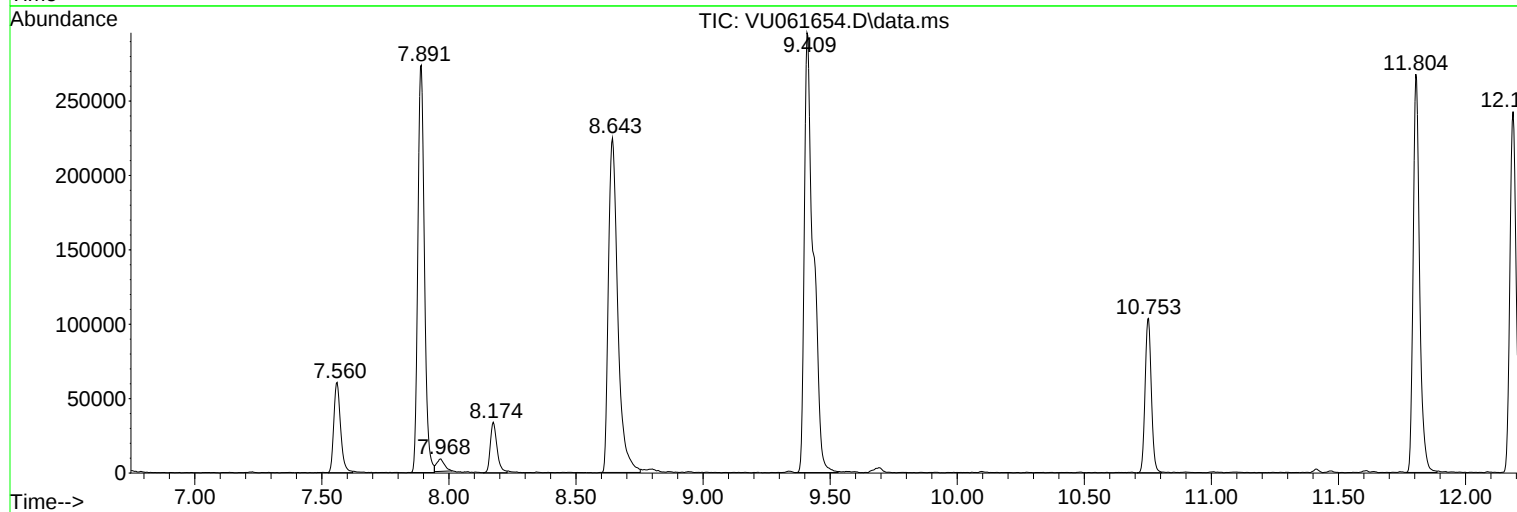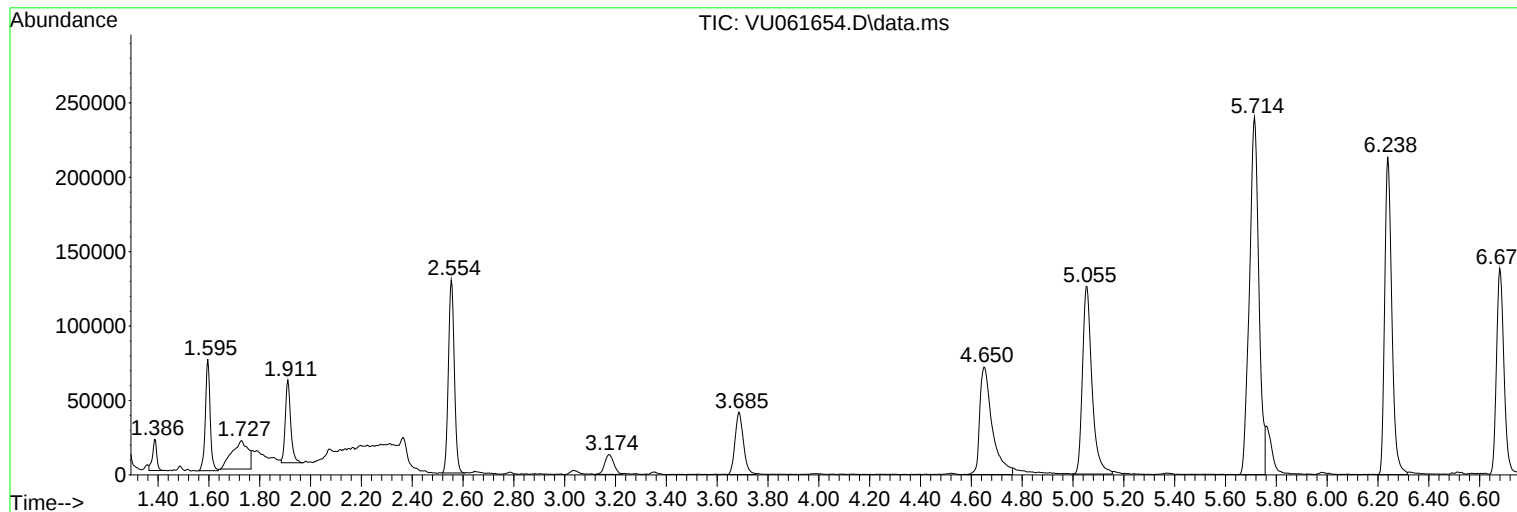

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
Data File : VU061654.D
Acq On : 14 Nov 2024 04:16
Operator : MD/SY
Sample : P4803-18 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Ethyl-oxetane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.685	1.15 ug/L	95991	1,4-Difluorobenzene	6.238

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Ethyl-oxetane	86	C5H10O	1010386-40-2	90
2	n-Hexane	86	C6H14	000110-54-3	72
3	n-Hexane	86	C6H14	000110-54-3	72
4	n-Hexane	86	C6H14	000110-54-3	64
5	n-Hexane	86	C6H14	000110-54-3	59

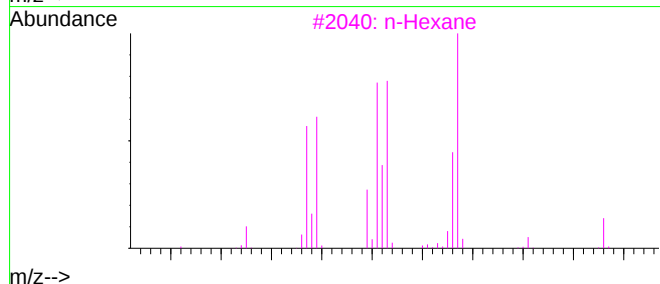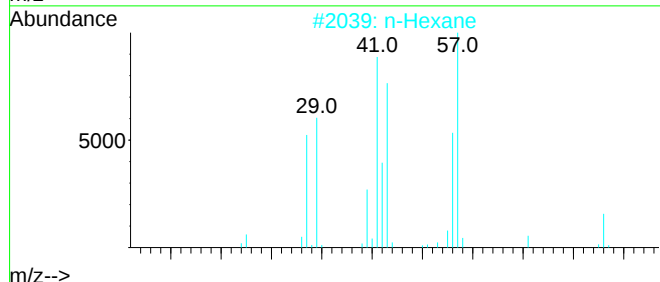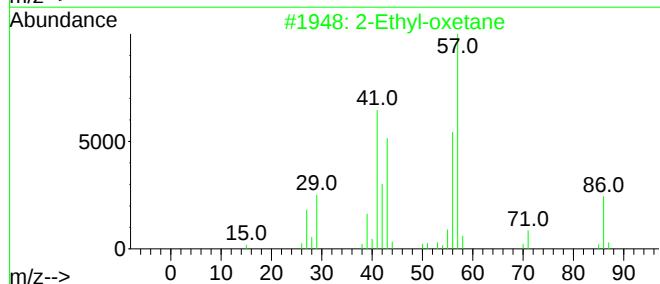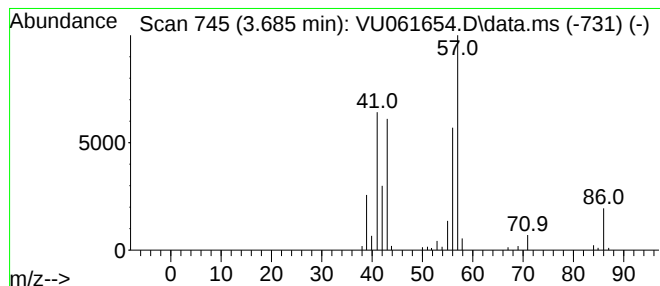

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111324\
Data File : VU061654.D
Acq On : 14 Nov 2024 04:16
Operator : MD/SY
Sample : P4803-18 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Ethyl-oxetane	3.685	1.1	ug/L	95991	1	6.238	417796	5.0