

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111424\
 Data File : VU061680.D
 Acq On : 14 Nov 2024 18:36
 Operator : MD/SY
 Sample : P4761-16
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AM0

Quant Time: Nov 15 00:49:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 15 00:40:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	172982	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	163671	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	73057	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	49952	4.469	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%
7) Chloroethane-d5	1.911	69	48445	5.077	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.600%
11) 1,1-Dichloroethene-d2	2.563	65	22431	4.473	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.400%
20) 2-Butanone-d5	4.624	46	118923	50.131	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.260%
24) Chloroform-d	5.052	84	103075	4.640	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	5.692	65	52896	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.718	84	220592	4.872	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	6.679	67	66345	4.968	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.891	98	195178	4.625	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
43) trans-1,3-Dichloroprop...	8.174	79	20788	4.226	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.627	63	95201	48.976	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.960%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	48820	4.637	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.800%
66) 1,2-Dichlorobenzene-d4	12.184	152	65898	5.064	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds					Qvalue	
13) Acetone	2.640	43	14078	9.419	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111424\
Data File : VU061680.D
Acq On : 14 Nov 2024 18:36
Operator : MD/SY
Sample : P4761-16
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AM0

Quant Time: Nov 15 00:49:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 15 00:40:52 2024
Response via : Initial Calibration

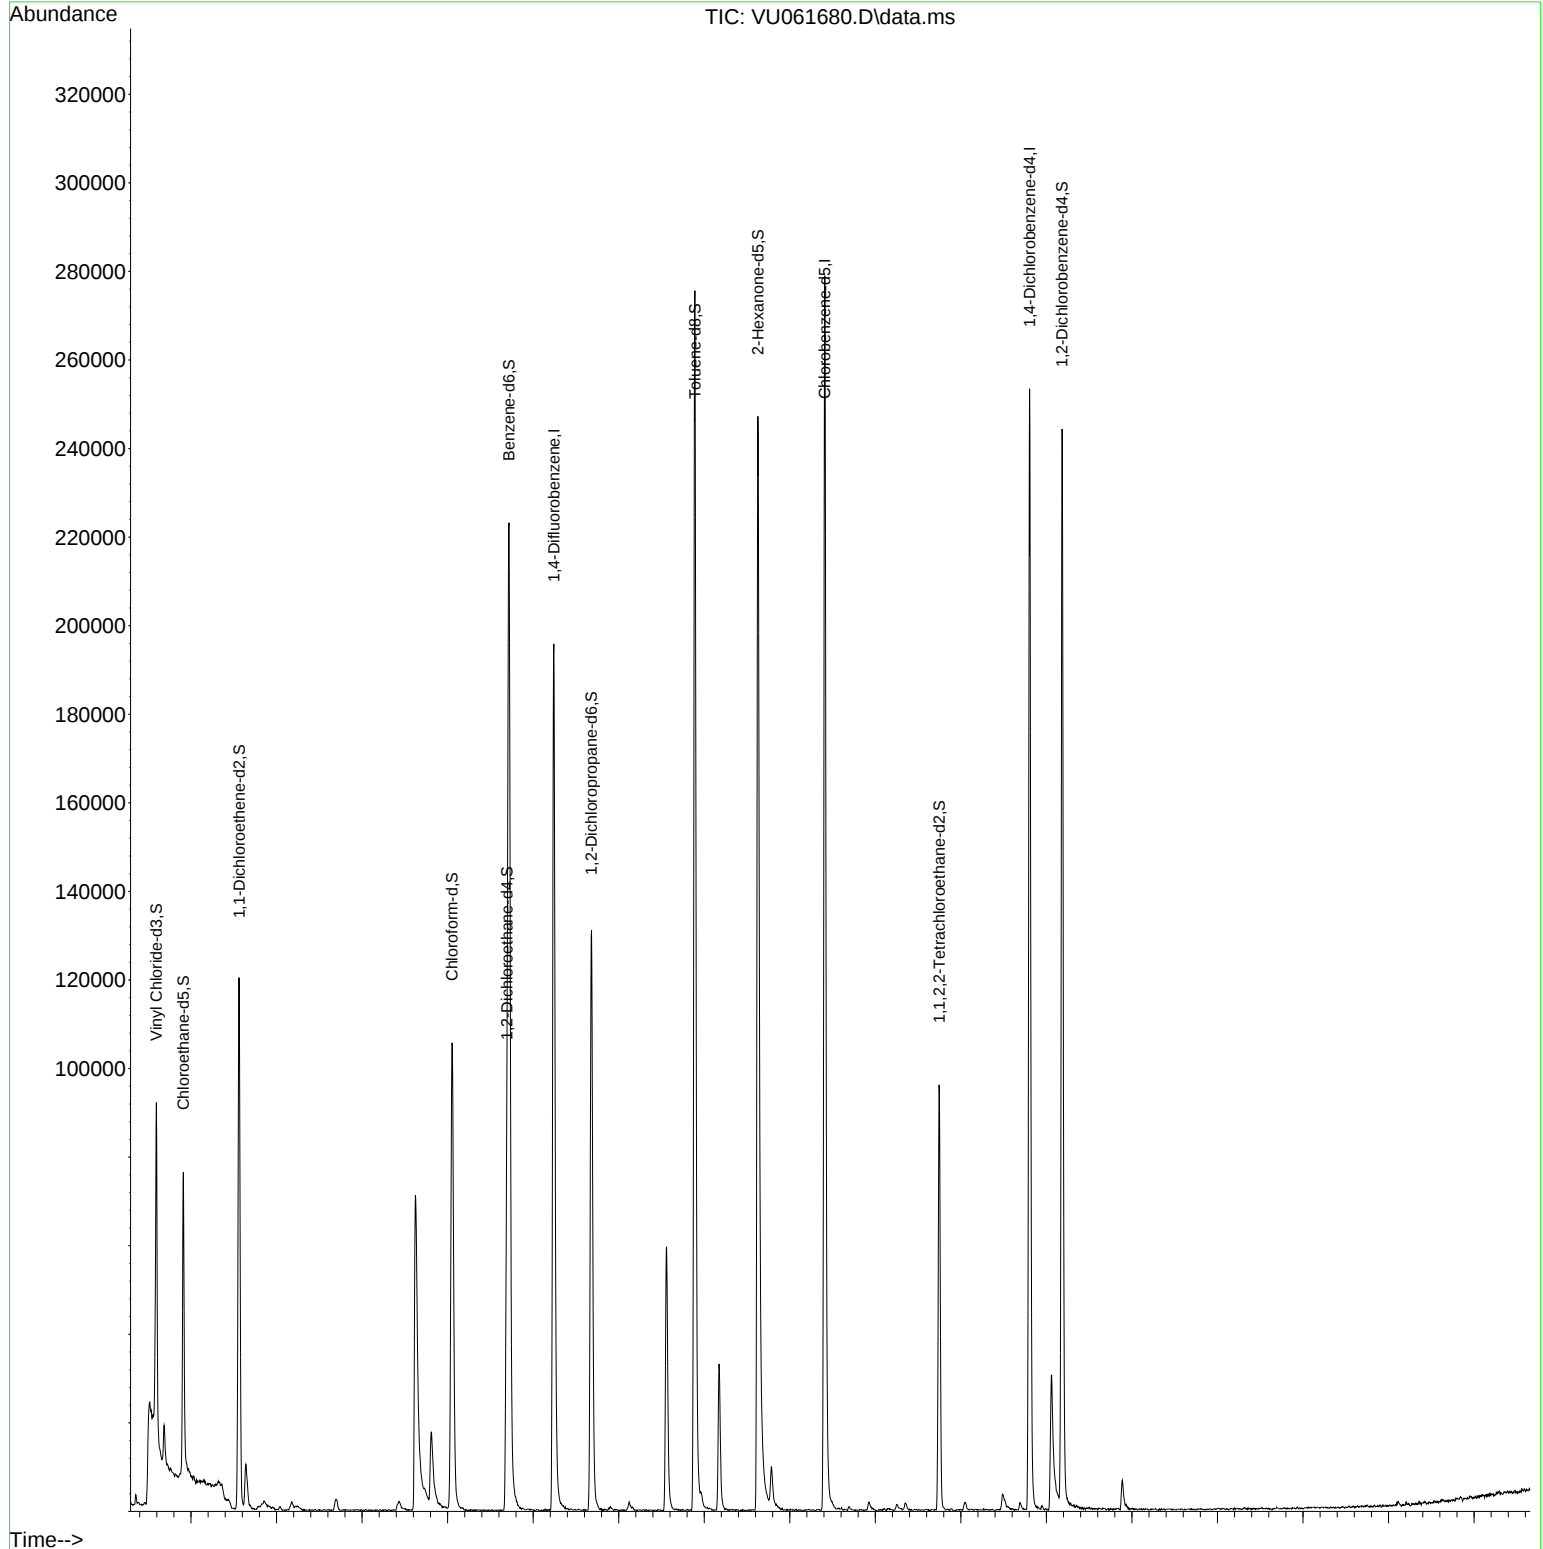

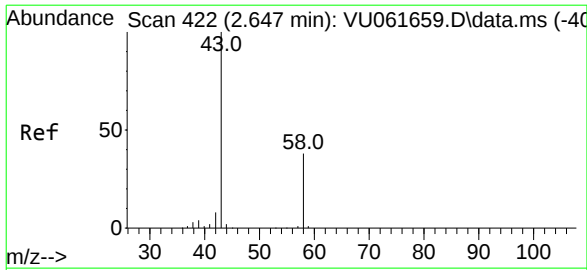

#13
 Acetone
 Concen: 9.419 ug/L
 RT: 2.640 min Scan# 42
 Delta R.T. -0.006 min
 Lab File: VU061680.D
 Acq: 14 Nov 2024 18:36

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AM0

Tgt Ion: 43 Resp: 14078
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 69.8

