

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111424\
 Data File : VU061688.D
 Acq On : 14 Nov 2024 22:40
 Operator : MD/SY
 Sample : P4803-04 2X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AP6

Quant Time: Nov 15 03:22:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 15 03:17:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	169177	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	152009	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	67054	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	48294	4.418	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.400%	
7) Chloroethane-d5	1.907	69	41929	4.493	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.800%	
11) 1,1-Dichloroethene-d2	2.550	65	22810	4.651	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.000%	
20) 2-Butanone-d5	4.663	46	96121	41.430	ug/L	0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	=	82.860%	
24) Chloroform-d	5.052	84	102390	4.713	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.692	65	52291	5.015	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.400%	
32) Benzene-d6	5.714	84	208152	4.950	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6	6.682	67	65642	5.292	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.800%	
41) Toluene-d8	7.888	98	172448	4.400	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.000%	
43) trans-1,3-Dichloroprop...	8.174	79	19233	4.210	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.200%	
46) 2-Hexanone-d5	8.640	63	102247	56.636	ug/L	0.01
Spiked Amount	50.000	Range 45 - 130	Recovery	=	113.280%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49417	5.054	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	12.187	152	58461	4.895	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.000%	
Target Compounds					Qvalue	
25) Chloroform	5.074	83	6007	0.279	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111424\
Data File : VU061688.D
Acq On : 14 Nov 2024 22:40
Operator : MD/SY
Sample : P4803-04 2X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0AP6

Quant Time: Nov 15 03:22:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 15 03:17:58 2024
Response via : Initial Calibration

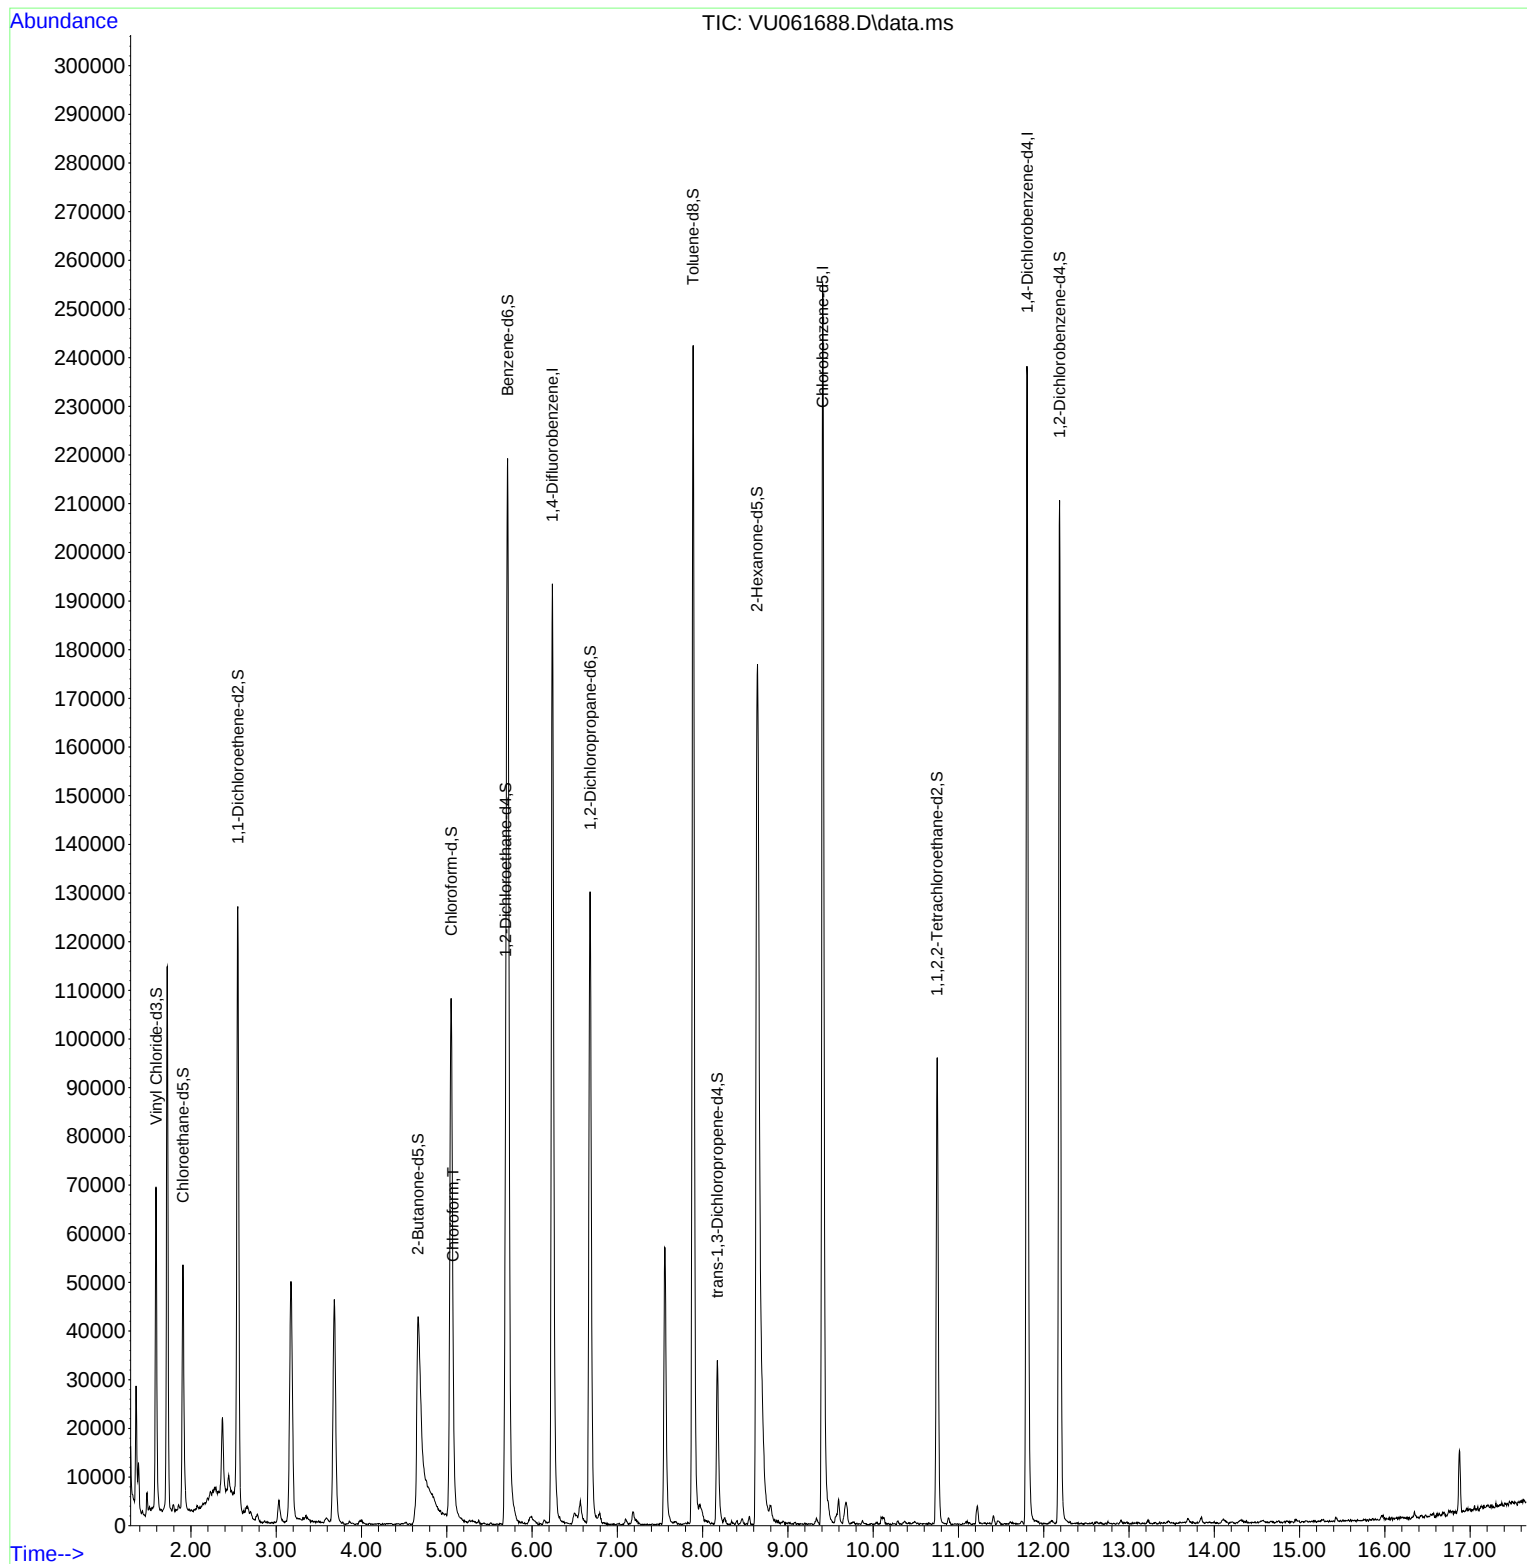

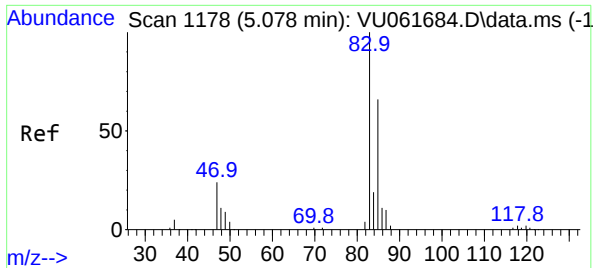

#25
 Chloroform
 Concen: 0.279 ug/L
 RT: 5.074 min Scan# 11
 Delta R.T. -0.003 min
 Lab File: VU061688.D
 Acq: 14 Nov 2024 22:40

Instrument :
 MSVOA_U
 ClientSampleId :
 A0AP6

Tgt Ion: 83 Resp: 6007
 Ion Ratio Lower Upper
 83 100
 85 68.7 44.1 81.9

