
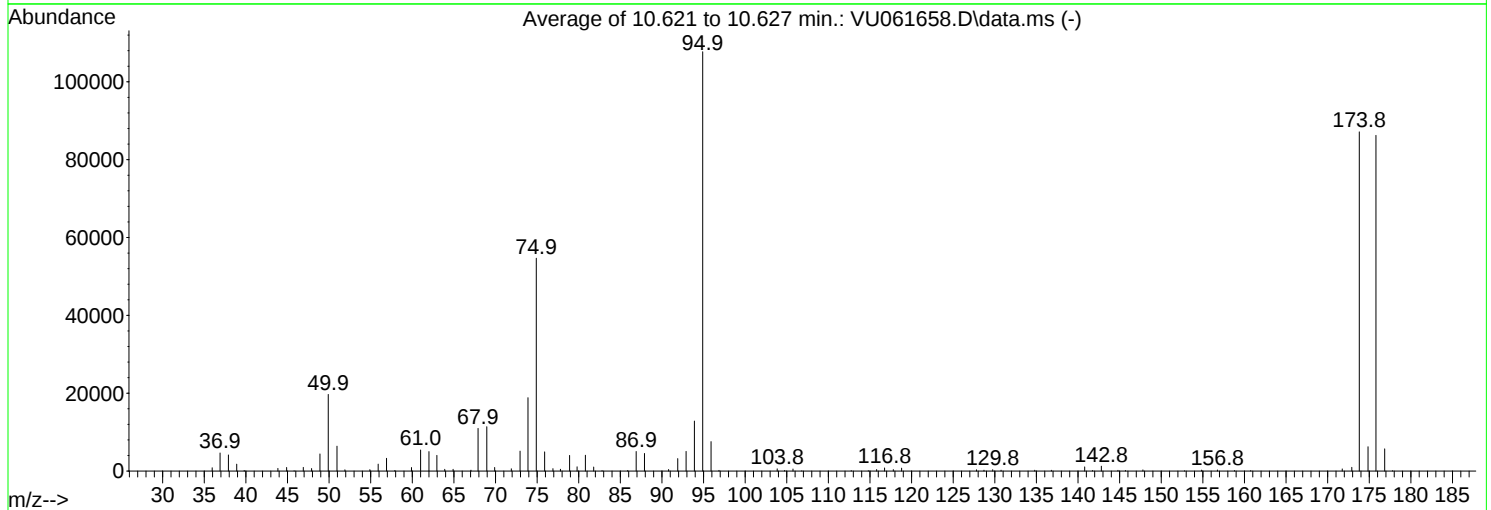


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111424\
Data File : VU061658.D
Acq On : 14 Nov 2024 08:44
Operator : MD/SY
Sample : BFB026
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB026

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 19 03:37:44 2024

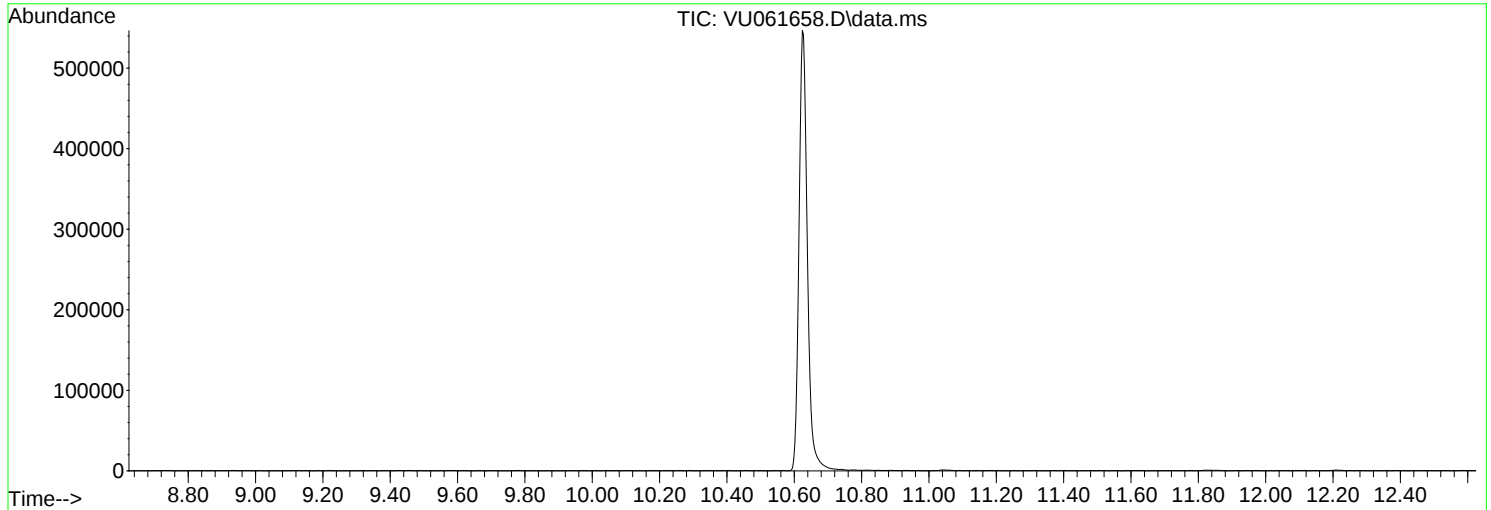

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	19691	PASS
75	95	30	80	50.8	54680	PASS
95	95	100	100	100.0	107728	PASS
96	95	5	9	7.0	7577	PASS
173	174	0.00	2	1.1	965	PASS
174	95	50	120	80.9	87144	PASS
175	174	5	9	7.2	6251	PASS
176	174	95	101	99.0	86240	PASS
177	176	5	9	6.6	5713	PASS

m/z	Abundance
43.70	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	848.0
36.90	4459.0
37.90	3931.0
38.90	1662.0
39.80	141.0
43.90	903.0
44.90	893.0
46.90	943.0
47.90	639.0
48.90	4189.0
49.90	19184.0
51.00	6040.0
51.90	292.0
54.90	348.0
55.90	1724.0
56.90	3167.0
57.90	145.0
59.90	888.0
61.00	5264.0
62.00	4724.0
62.90	3903.0
63.90	458.0
64.90	427.0
67.00	256.0
67.90	10884.0
68.90	11055.0
69.90	921.0
71.90	596.0
73.00	5102.0
73.90	18224.0
74.90	52776.0
75.90	4723.0
76.90	591.0
77.80	432.0
78.90	3898.0
79.80	1048.0
80.80	3915.0
81.80	991.0
82.70	113.0
85.80	129.0
86.90	4682.0
87.90	4229.0
90.80	380.0
91.90	3048.0
92.90	4630.0
93.90	12194.0
94.90	103008.0
95.90	7453.0
96.90	200.0
103.90	549.0
104.70	160.0
105.80	479.0
106.80	110.0
112.80	127.0
115.80	398.0
116.80	695.0
117.70	368.0
118.80	750.0
127.80	328.0
128.70	227.0
129.70	366.0
130.80	239.0
134.80	207.0
136.80	191.0
140.80	916.0
141.80	138.0
142.80	1249.0
144.80	196.0
145.70	141.0
147.80	243.0
152.80	122.0
154.90	202.0
156.70	281.0
158.80	110.0
160.80	139.0
171.80	543.0
172.90	947.0
173.80	80584.0
174.80	5992.0
175.80	79744.0
176.80	5470.0
177.80	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	877.0
36.90	4764.0
37.90	4277.0
38.90	1851.0
39.80	153.0
43.90	918.0
44.90	982.0
45.80	108.0
46.90	976.0
47.90	682.0
48.90	4546.0
49.90	20352.0
50.90	6641.0
51.90	336.0
54.90	378.0
55.90	1858.0
56.90	3387.0
57.90	161.0
59.90	938.0
61.00	5648.0
62.00	5100.0
62.90	4193.0
63.90	474.0
64.90	478.0
67.10	249.0
67.90	11319.0
68.90	11750.0
69.90	956.0
71.90	610.0
73.00	5290.0
73.90	19400.0
74.90	56152.0
75.90	5081.0
76.90	652.0
77.80	505.0
78.90	4143.0
79.80	1134.0
80.80	4193.0
81.80	1059.0
82.80	135.0
85.90	144.0
86.90	5259.0
87.90	4625.0
90.80	437.0
91.90	3296.0
92.90	5291.0
93.90	13185.0
94.90	110824.0
95.90	7840.0
96.80	182.0
103.80	616.0
104.70	183.0
105.70	550.0
106.80	103.0
112.70	133.0
114.80	137.0
115.80	400.0
116.80	823.0
117.80	381.0
118.80	795.0
127.80	347.0
128.70	255.0
129.80	365.0
130.70	253.0
134.80	238.0
136.80	222.0
140.80	1106.0
141.80	165.0
142.80	1297.0
144.80	210.0
145.70	156.0
147.80	313.0
152.80	121.0
154.90	262.0
156.80	308.0
158.80	143.0
160.70	118.0
171.70	574.0
172.90	1002.0
173.80	89680.0
174.80	6446.0
175.80	89000.0
176.80	5933.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	818.0
36.90	4742.0
37.90	4240.0
38.90	1821.0
39.80	194.0
43.90	864.0
44.90	918.0
45.80	134.0
46.90	955.0
47.90	630.0
48.90	4493.0
49.90	19536.0
50.90	6535.0
51.90	356.0
54.90	378.0
55.90	1772.0
56.90	3303.0
57.90	139.0
59.90	908.0
61.00	5318.0
62.00	5206.0
63.00	4012.0
63.90	439.0
64.90	465.0
67.00	225.0
67.90	10685.0
69.00	11394.0
69.90	900.0
71.90	585.0
72.90	5004.0
73.90	18952.0
74.90	55112.0
75.90	4985.0
76.90	645.0
77.80	488.0
78.90	4011.0
79.80	1100.0
80.80	4113.0
81.80	1051.0
82.90	117.0
85.80	115.0
86.90	5146.0
87.90	4714.0
90.80	425.0
91.90	3289.0
92.90	5252.0
93.90	13154.0
94.90	109352.0
95.90	7437.0
96.80	180.0
103.80	587.0
104.80	187.0
105.70	584.0
112.70	129.0
114.80	162.0
115.80	385.0
116.70	877.0
117.90	394.0
118.80	717.0
127.80	331.0
128.70	228.0
129.80	336.0
130.70	219.0
134.80	216.0
136.80	226.0
140.80	1188.0
141.70	163.0
142.80	1243.0
144.80	194.0
145.70	161.0
147.80	373.0
154.80	276.0
156.80	257.0
158.80	142.0
160.70	105.0
171.80	542.0
172.90	946.0
173.80	91168.0
174.90	6316.0
175.80	89976.0
176.90	5736.0
177.80	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026