
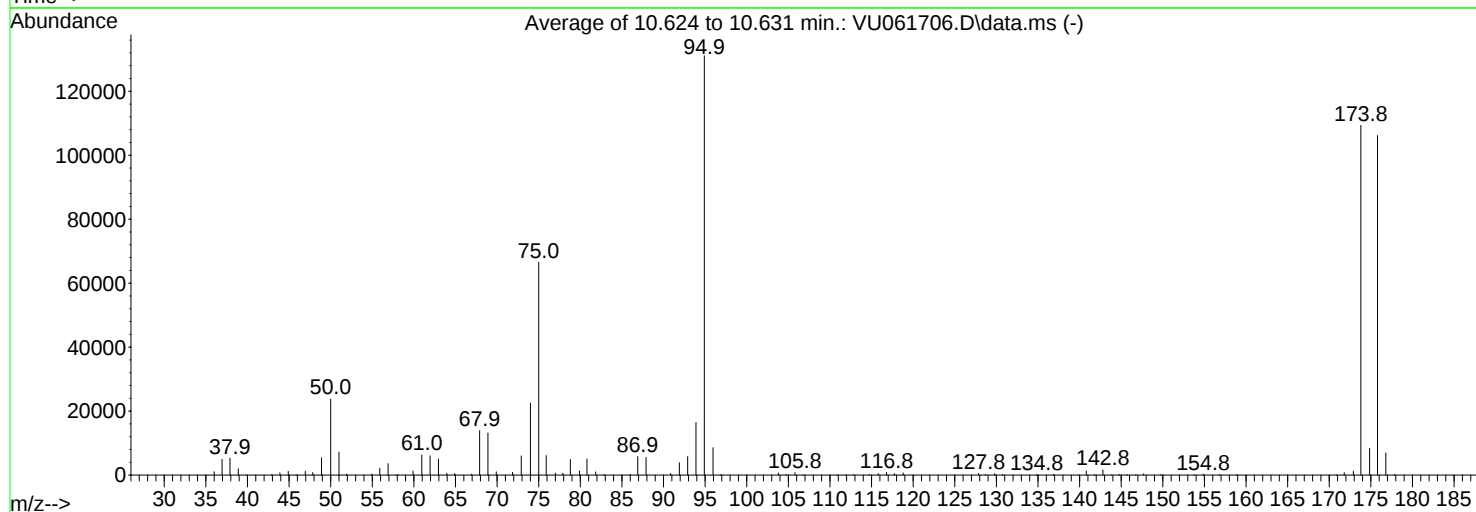


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111524\
Data File : VU061706.D
Acq On : 15 Nov 2024 08:18
Operator : MD/SY
Sample : BFB027
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB027

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 18 04:15:29 2024

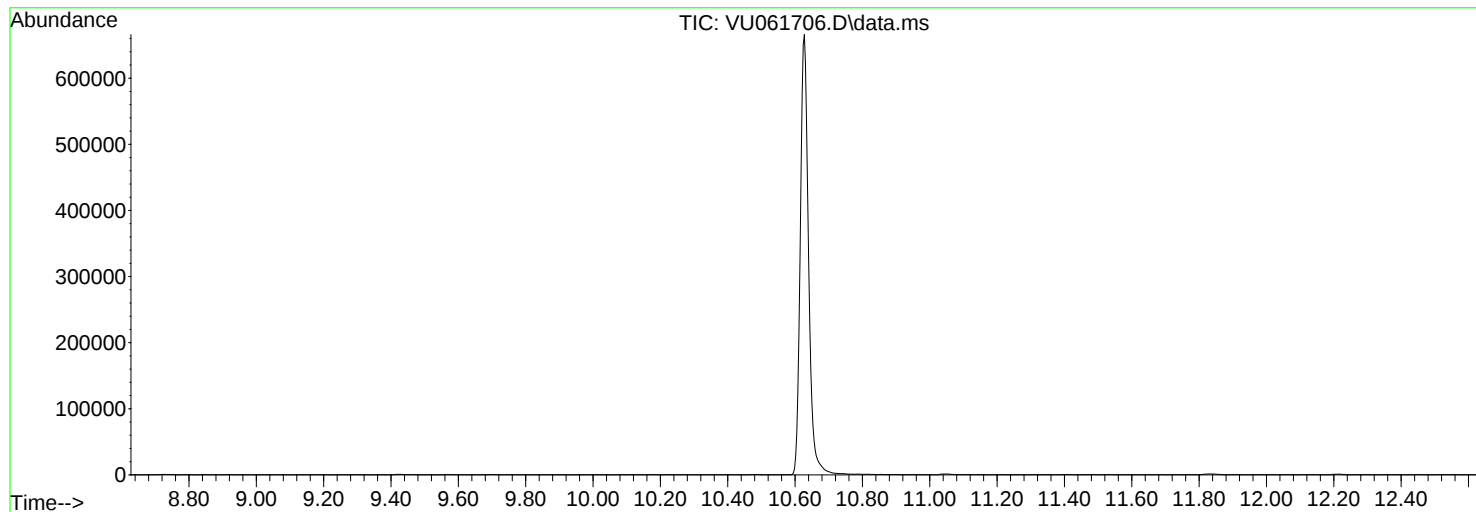

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	23792	PASS
75	95	30	80	50.8	66552	PASS
95	95	100	100	100.0	131109	PASS
96	95	5	9	6.5	8577	PASS
173	174	0.00	2	1.1	1192	PASS
174	95	50	120	83.4	109349	PASS
175	174	5	9	7.6	8325	PASS
176	174	95	101	97.1	106152	PASS
177	176	5	9	6.5	6929	PASS

Scan 2890 (10.582 min): VU061706.D\data.ms
BFB027

m/z	Abundance
39.80	114.0
43.90	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	1015.0
37.00	5028.0
37.90	5247.0
38.90	1891.0
39.80	156.0
43.90	916.0
44.90	1203.0
45.80	107.0
46.90	1180.0
47.80	786.0
48.90	5512.0
50.00	24416.0
51.00	7672.0
51.90	321.0
55.00	340.0
55.90	2159.0
56.90	3679.0
57.80	206.0
59.90	1324.0
60.90	6463.0
62.00	6210.0
62.90	5252.0
64.00	546.0
64.90	508.0
66.90	305.0
67.90	14028.0
68.90	13475.0
69.90	1073.0
71.90	877.0
72.90	6161.0
74.00	23072.0
75.00	68208.0
75.90	6419.0
77.00	761.0
77.90	688.0
78.80	5030.0
79.90	1308.0
80.80	5132.0
81.80	1007.0
82.90	144.0
86.00	235.0
86.90	5711.0
87.90	5678.0
90.80	500.0
91.90	3890.0
92.90	5892.0
93.90	16376.0
94.90	132032.0
96.00	8836.0
96.90	195.0
103.80	641.0
104.80	182.0
105.80	763.0
106.80	135.0
110.80	123.0
111.90	107.0
112.80	128.0
114.70	100.0
115.70	524.0
116.80	819.0
117.70	464.0
118.80	715.0
127.80	509.0
128.70	229.0
129.80	477.0
130.80	212.0
134.80	156.0
136.90	212.0
140.80	1348.0
141.80	183.0
142.80	1790.0
143.80	119.0
144.80	295.0
145.70	185.0
146.70	106.0
147.70	355.0
149.70	145.0
153.80	110.0
154.90	288.0
156.80	191.0
158.90	202.0
170.90	119.0
171.80	759.0
172.90	1054.0
173.80	108416.0
174.90	8217.0
175.80	103960.0
176.80	6904.0
177.80	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	1106.0
37.00	5056.0
37.90	5543.0
38.90	2028.0
39.80	158.0
42.90	113.0
43.90	974.0
44.90	1282.0
45.90	101.0
47.00	1249.0
47.80	818.0
48.90	5618.0
50.00	24520.0
51.00	7355.0
51.90	318.0
54.90	336.0
55.90	2260.0
56.90	3691.0
57.90	147.0
59.90	1369.0
61.00	6523.0
62.00	6214.0
62.90	5130.0
64.00	555.0
64.90	488.0
66.90	267.0
67.90	14390.0
68.90	13468.0
69.90	1026.0
71.90	886.0
72.90	6148.0
74.00	23008.0
75.00	68296.0
75.90	6298.0
77.00	697.0
77.90	605.0
78.80	4976.0
79.90	1358.0
80.80	5267.0
81.90	1029.0
82.80	173.0
86.00	221.0
86.90	6023.0
87.90	5726.0
90.80	540.0
91.90	3987.0
92.90	5895.0
93.90	16976.0
94.90	135104.0
95.90	8743.0
96.90	151.0
103.80	641.0
104.70	201.0
105.80	781.0
106.80	118.0
110.80	117.0
111.90	103.0
112.80	122.0
114.70	154.0
115.80	509.0
116.80	857.0
117.70	467.0
118.80	673.0
127.90	507.0
128.70	246.0
129.80	481.0
130.80	192.0
134.80	174.0
136.80	244.0
140.80	1364.0
141.80	156.0
142.80	1700.0
144.70	267.0
145.70	192.0
146.80	122.0
147.70	429.0
149.80	138.0
153.70	126.0
154.80	309.0
156.80	209.0
158.90	172.0
170.90	118.0
171.80	775.0
172.90	1241.0
173.80	112480.0
174.80	8591.0
175.80	109408.0
176.80	7108.0
177.90	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	1018.0
36.90	4691.0
37.90	5125.0
38.90	1975.0
39.80	168.0
42.90	105.0
43.90	996.0
44.90	1133.0
45.90	129.0
47.00	1190.0
47.90	812.0
48.90	5096.0
50.00	22440.0
51.00	6601.0
51.90	265.0
54.90	335.0
55.90	2061.0
56.90	3427.0
58.10	129.0
59.90	1169.0
61.00	5831.0
61.90	5634.0
63.00	4674.0
63.90	571.0
64.90	453.0
66.90	229.0
67.90	13245.0
68.90	12562.0
69.90	953.0
71.80	799.0
72.90	5703.0
74.00	21464.0
75.00	63152.0
75.90	5594.0
77.00	548.0
77.90	495.0
78.80	4565.0
79.90	1286.0
80.80	4744.0
81.90	983.0
82.80	167.0
86.00	196.0
86.90	5617.0
87.90	5248.0
90.90	510.0
91.90	3695.0
92.90	5534.0
93.90	15910.0
94.90	126192.0
95.90	8153.0
96.90	129.0
103.80	634.0
104.70	177.0
105.80	715.0
106.80	102.0
110.90	111.0
112.80	111.0
114.70	177.0
115.90	460.0
116.80	835.0
117.80	471.0
118.80	646.0
127.90	520.0
128.70	219.0
129.80	464.0
130.70	175.0
134.90	170.0
136.80	264.0
139.80	102.0
140.80	1299.0
141.80	122.0
142.80	1364.0
144.70	199.0
145.70	187.0
146.80	119.0
147.70	452.0
149.80	127.0
153.70	109.0
154.80	350.0
156.80	189.0
158.80	114.0
170.80	121.0
171.80	702.0
172.90	1281.0
173.80	107152.0
174.80	8166.0
175.80	105088.0
176.80	6775.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027