

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111724\
 Data File : VU061781.D
 Acq On : 17 Nov 2024 13:45
 Operator : MD/SY
 Sample : P4800-18DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCPB7DL

Quant Time: Nov 18 00:05:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 18 00:04:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	192700	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	182422	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	82168	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	38490	3.091	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.800%
7) Chloroethane-d5	1.908	69	48734	4.585	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.551	65	20275	3.629	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	4.634	46	119880	45.363	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.720%
24) Chloroform-d	5.052	84	100722	4.070	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.400%
26) 1,2-Dichloroethane-d4	5.692	65	52496	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.400%
32) Benzene-d6	5.714	84	205520	4.072	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.400%
36) 1,2-Dichloropropane-d6	6.679	67	64500	4.333	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.600%
41) Toluene-d8	7.891	98	184570	3.924	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	8.177	79	19025	3.470	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.400%
46) 2-Hexanone-d5	8.644	63	106350	49.088	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.180%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	50713	4.322	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	63408	4.333	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds					Qvalue	
13) Acetone	2.644	43	72039	43.268	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111724\
Data File : VU061781.D
Acq On : 17 Nov 2024 13:45
Operator : MD/SY
Sample : P4800-18DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCPB7DL

Quant Time: Nov 18 00:05:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 18 00:04:27 2024
Response via : Initial Calibration

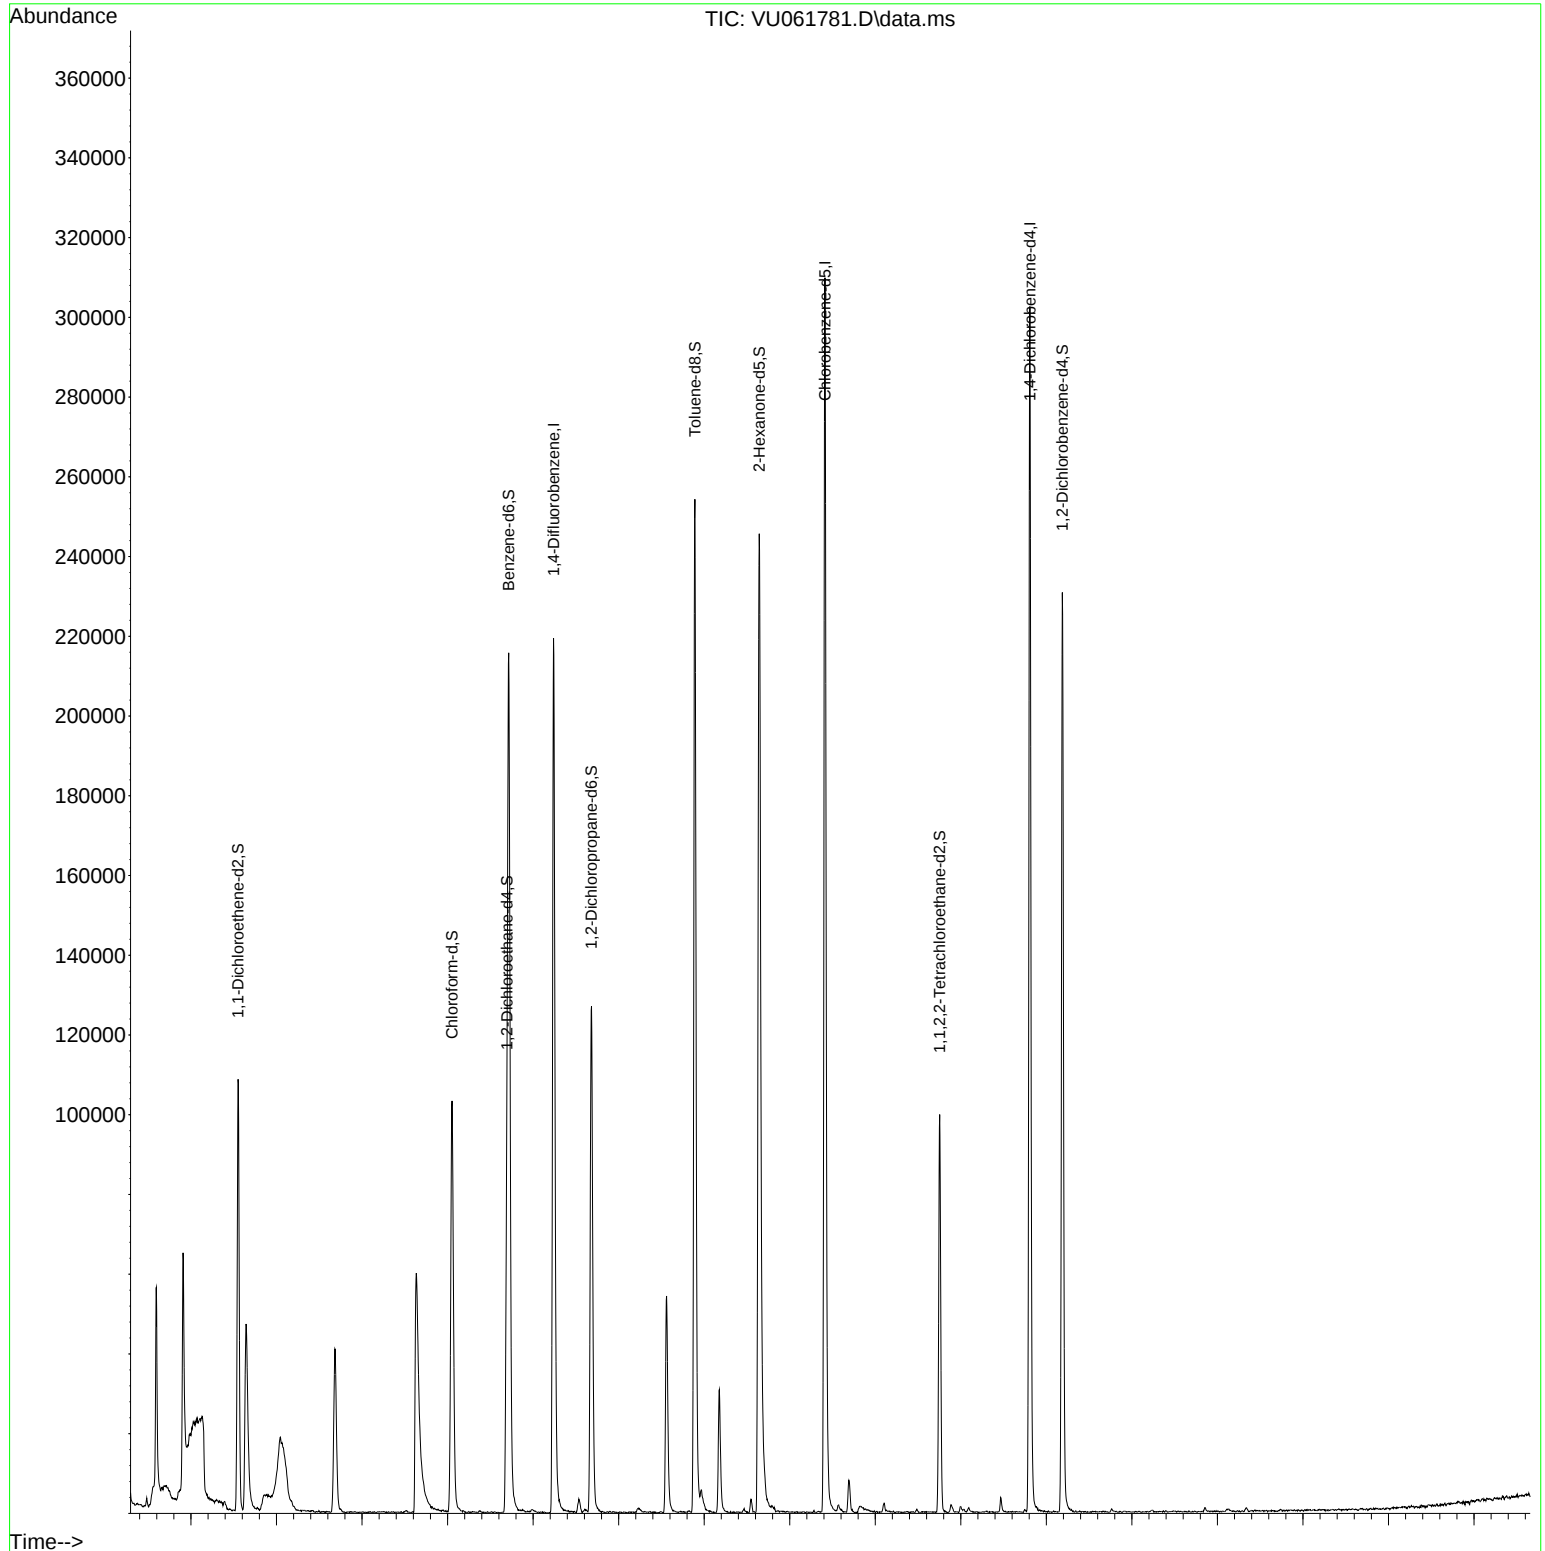

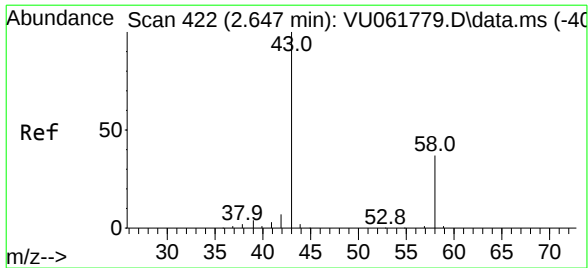

#13
 Acetone
 Concen: 43.268 ug/L
 RT: 2.644 min Scan# 42
 Delta R.T. -0.003 min
 Lab File: VU061781.D
 Acq: 17 Nov 2024 13:45

Instrument :
 MSVOA_U
 ClientSampleId :
 GCPB7DL

Tgt Ion: 43 Resp: 72039
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 69.8

