
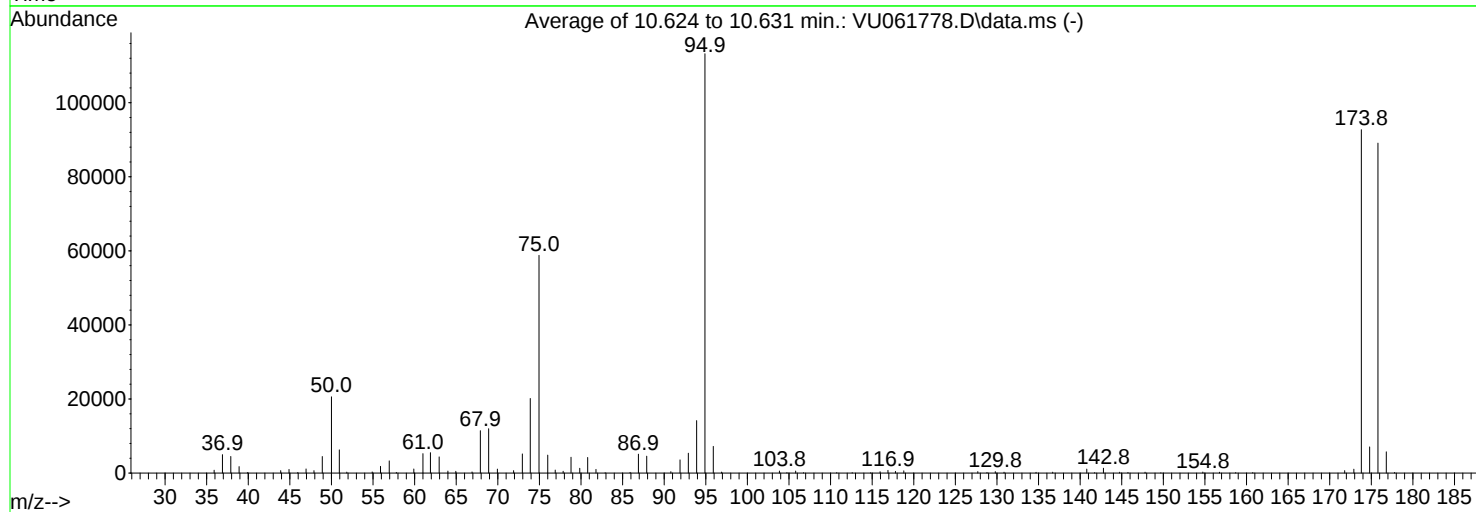


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111724\
Data File : VU061778.D
Acq On : 17 Nov 2024 11:10
Operator : MD/SY
Sample : BFB029
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB029

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 18 04:15:29 2024

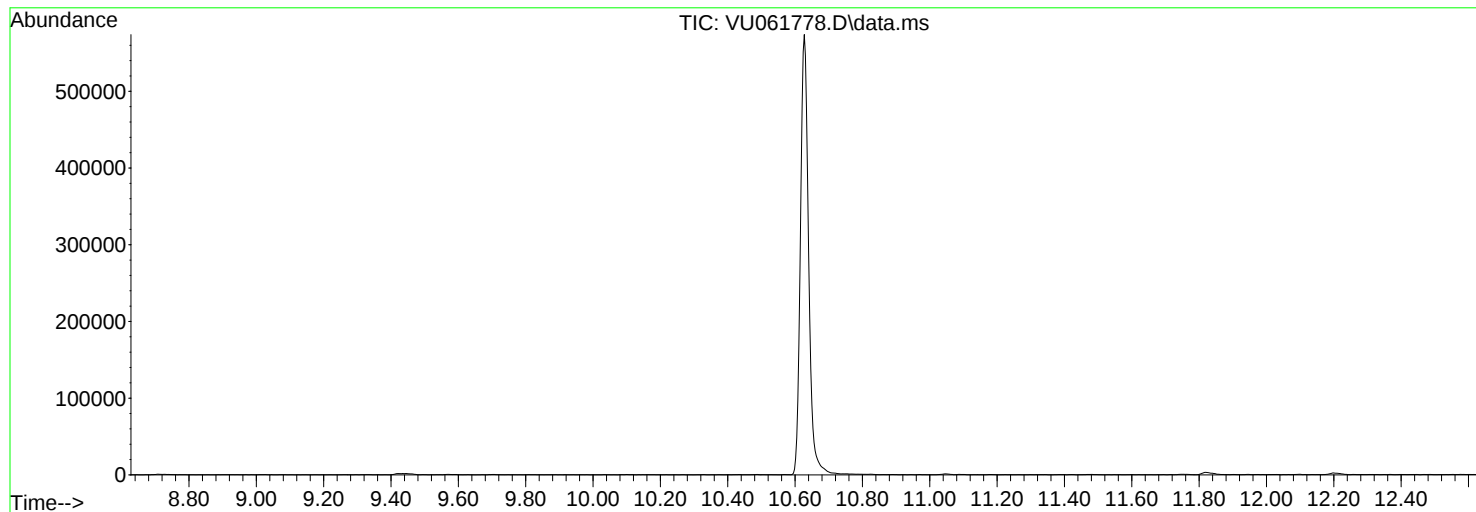

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	20600	PASS
75	95	30	80	51.9	58795	PASS
95	95	100	100	100.0	113229	PASS
96	95	5	9	6.4	7215	PASS
173	174	0.00	2	1.1	1050	PASS
174	95	50	120	81.9	92720	PASS
175	174	5	9	7.6	7066	PASS
176	174	95	101	96.1	89093	PASS
177	176	5	9	6.4	5737	PASS

m/z	Abundance
43.90	288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
35.90	812.0
36.90	4974.0
37.90	4520.0
38.90	1744.0
39.90	171.0
44.00	933.0
44.90	1042.0
45.90	149.0
47.00	1138.0
47.90	714.0
48.90	4606.0
50.00	20864.0
51.00	6469.0
51.80	266.0
54.90	334.0
55.90	1773.0
56.90	3430.0
57.80	229.0
59.90	1160.0
61.00	5501.0
61.90	5606.0
63.00	4345.0
64.00	538.0
64.90	468.0
66.90	342.0
67.90	11466.0
68.90	12019.0
69.90	1115.0
71.90	707.0
73.00	5247.0
73.90	20176.0
74.90	58440.0
76.00	4902.0
76.90	843.0
77.90	441.0
78.80	4281.0
79.80	1294.0
80.80	4197.0
81.80	1024.0
85.90	154.0
86.90	5035.0
87.90	4708.0
90.80	362.0
91.90	3413.0
92.90	5328.0
93.90	14147.0
94.90	111920.0
95.90	7284.0
96.90	246.0
103.90	561.0
104.80	157.0
105.80	643.0
106.70	110.0
110.70	116.0
112.60	115.0
114.80	154.0
115.90	381.0
116.90	678.0
117.80	419.0
118.80	585.0
127.70	418.0
128.80	180.0
129.80	402.0
130.80	185.0
134.70	215.0
136.70	242.0
140.80	1035.0
141.70	116.0
142.80	1284.0
144.80	259.0
145.70	150.0
147.80	250.0
154.80	316.0
156.80	273.0
158.70	126.0
160.80	108.0
171.80	606.0
172.90	1003.0
173.80	90112.0
174.80	6948.0
175.80	86448.0
176.80	5790.0
177.80	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
35.90	804.0
36.90	5156.0
37.90	4609.0
38.90	1776.0
39.90	152.0
43.90	988.0
44.90	1024.0
46.00	147.0
46.90	1145.0
47.90	683.0
48.90	4599.0
50.00	21144.0
51.00	6453.0
51.80	268.0
54.90	314.0
55.90	1841.0
56.90	3390.0
57.80	197.0
59.90	1127.0
61.00	5368.0
61.90	5683.0
62.90	4485.0
64.00	551.0
65.00	489.0
66.90	322.0
67.90	11798.0
68.90	12315.0
70.00	1120.0
71.90	688.0
73.00	5283.0
73.90	20864.0
75.00	60472.0
76.00	4950.0
76.90	834.0
77.80	509.0
78.80	4394.0
79.90	1312.0
80.80	4337.0
81.80	1042.0
82.90	116.0
85.90	205.0
86.90	5279.0
87.90	4701.0
90.80	406.0
91.90	3677.0
92.90	5539.0
93.90	14553.0
94.90	116536.0
95.90	7398.0
96.90	279.0
103.90	565.0
104.80	124.0
105.80	552.0
106.70	108.0
110.70	153.0
112.60	130.0
114.80	107.0
116.00	384.0
116.90	768.0
117.80	461.0
118.80	628.0
127.70	392.0
128.80	175.0
129.80	419.0
130.90	262.0
134.70	208.0
136.70	265.0
140.80	1099.0
141.80	131.0
142.80	1348.0
144.80	224.0
145.70	184.0
147.80	254.0
149.70	109.0
154.70	292.0
156.70	233.0
158.70	158.0
160.70	151.0
171.80	663.0
172.90	1120.0
173.80	95600.0
174.80	7307.0
175.80	91944.0
176.80	5888.0
177.80	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
35.90	746.0
36.90	4795.0
37.90	4330.0
38.90	1713.0
39.90	112.0
43.90	941.0
44.90	908.0
46.00	134.0
46.90	1079.0
47.90	601.0
48.90	4219.0
50.00	19792.0
50.90	5901.0
51.90	255.0
54.90	298.0
55.90	1827.0
57.00	3055.0
57.90	129.0
59.90	1010.0
61.00	4871.0
61.90	5240.0
62.90	4274.0
64.00	539.0
65.00	499.0
66.90	260.0
67.90	11063.0
68.90	11608.0
70.00	999.0
71.90	605.0
72.90	4989.0
73.90	19368.0
75.00	57472.0
76.00	4706.0
76.90	782.0
77.80	536.0
78.80	4171.0
79.90	1292.0
80.80	4109.0
81.80	923.0
82.90	111.0
85.90	220.0
86.90	5021.0
87.90	4296.0
90.80	390.0
91.90	3605.0
92.90	5225.0
93.90	13798.0
94.90	111232.0
95.90	6964.0
96.90	295.0
103.80	560.0
104.70	124.0
105.80	426.0
106.80	106.0
110.80	158.0
112.60	108.0
115.90	360.0
116.90	772.0
117.80	465.0
118.80	640.0
127.70	380.0
128.80	145.0
129.80	407.0
130.90	298.0
134.70	210.0
136.70	238.0
140.80	1092.0
141.80	148.0
142.80	1311.0
144.70	208.0
145.80	192.0
147.80	253.0
149.70	130.0
154.70	248.0
156.70	180.0
158.70	156.0
160.70	193.0
171.80	698.0
172.90	1027.0
173.80	92448.0
174.80	6943.0
175.80	88888.0
176.80	5533.0
177.80	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029