

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
 Data File : VU061813.D
 Acq On : 18 Nov 2024 15:15
 Operator : MD/SY
 Sample : P4829-09
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E29W1

Quant Time: Nov 19 00:19:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 00:15:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	199216	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	192695	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	83594	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	45755	3.555	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.000%
7) Chloroethane-d5	1.907	69	44254	4.027	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	2.560	65	21385	3.703	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.000%
20) 2-Butanone-d5	4.608	46	136131	49.828	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.660%
24) Chloroform-d	5.052	84	116191	4.541	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
26) 1,2-Dichloroethane-d4	5.692	65	59013	4.806	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.718	84	233848	4.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	6.679	67	73199	4.656	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.891	98	204668	4.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	8.174	79	23547	4.066	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.621	63	110825	48.426	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.860%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	61282	4.944	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	73343	4.926	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds					Qvalue	
13) Acetone	2.618	43	24857	14.441	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061813.D
Acq On : 18 Nov 2024 15:15
Operator : MD/SY
Sample : P4829-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E29W1


Quant Time: Nov 19 00:19:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 00:15:47 2024
Response via : Initial Calibration

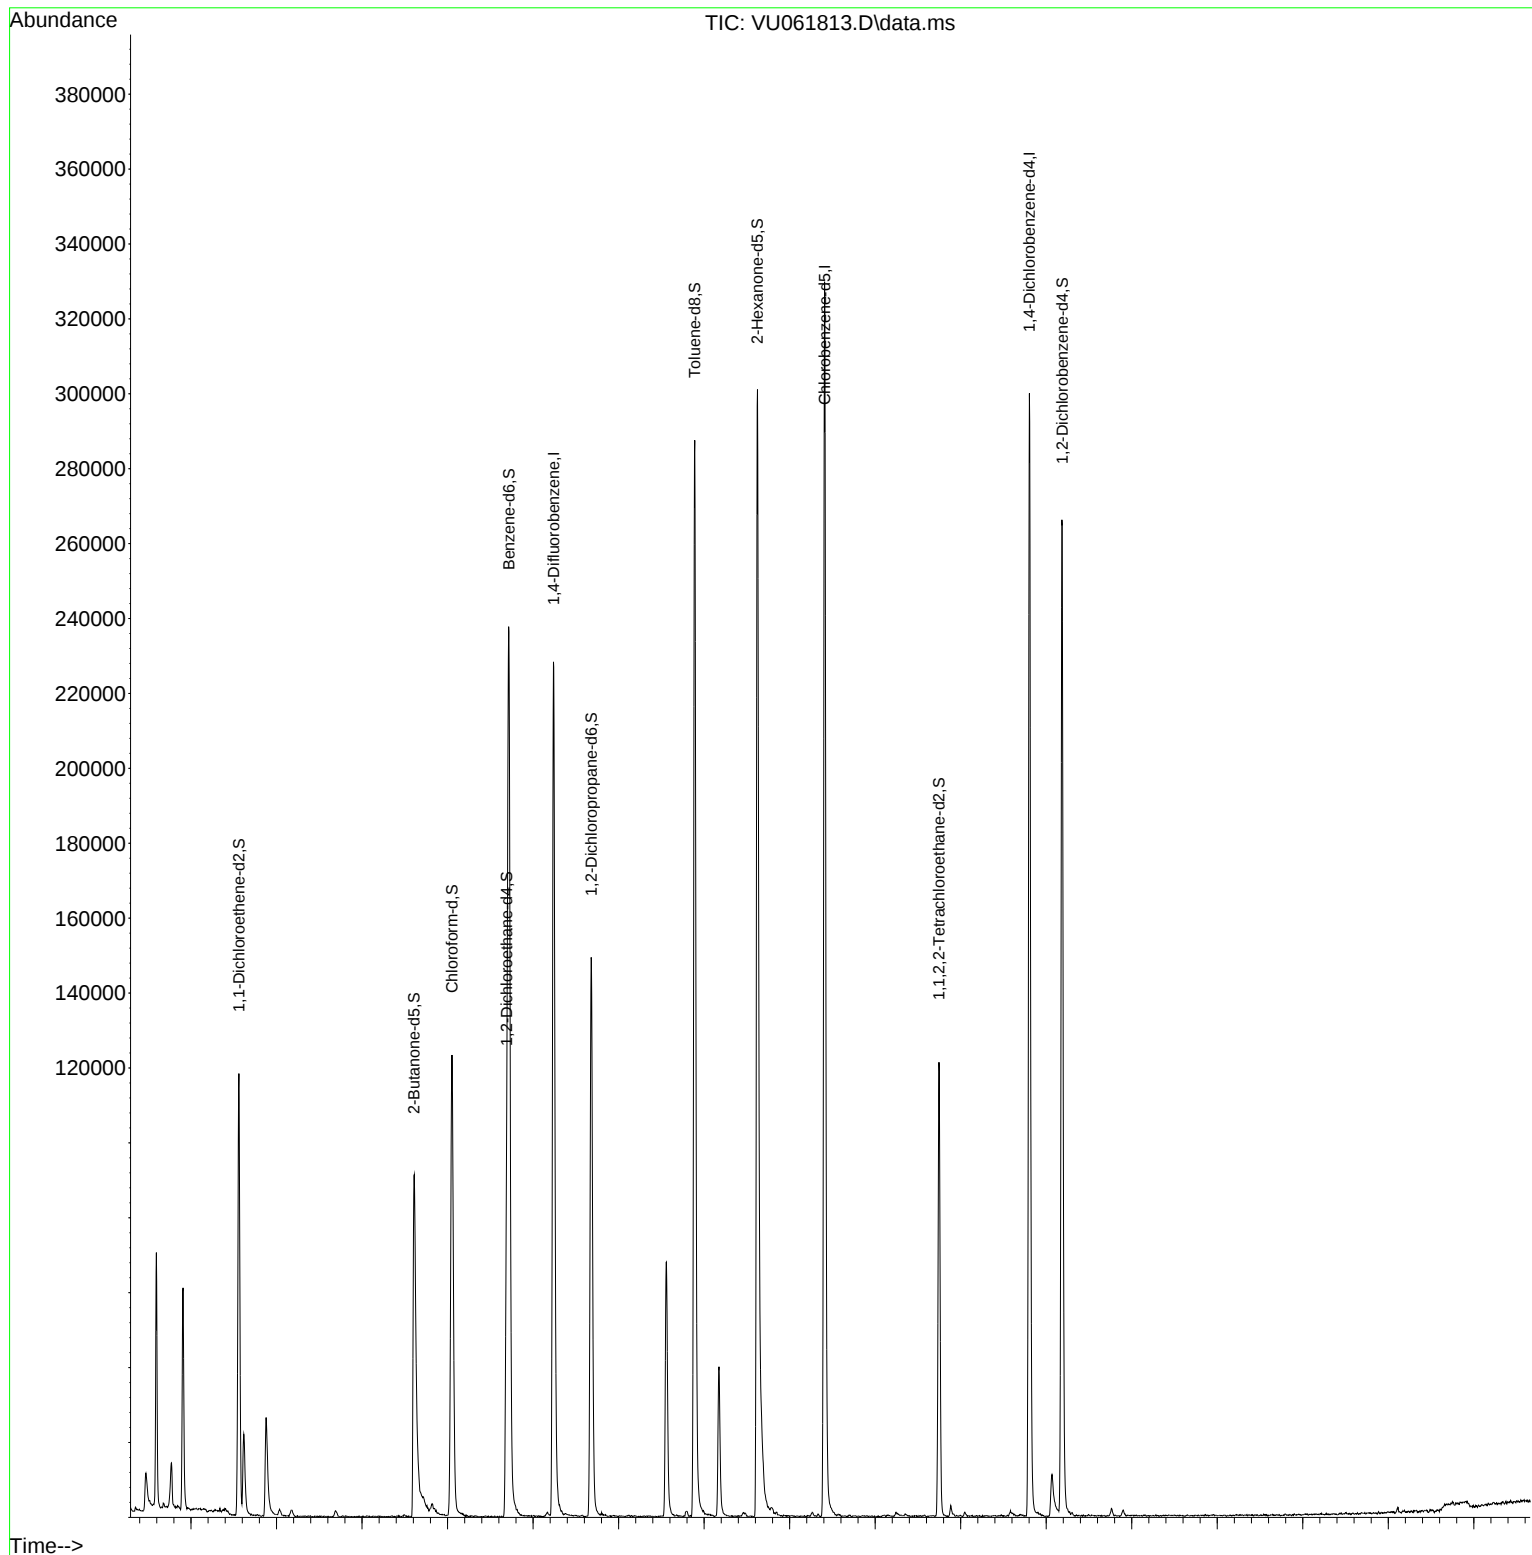

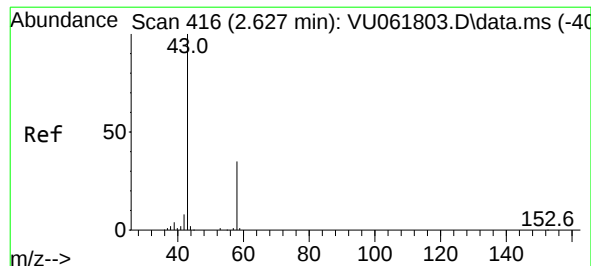

#13
 Acetone
 Concen: 14.441 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. -0.010 min
 Lab File: VU061813.D
 Acq: 18 Nov 2024 15:15

Instrument :
 MSVOA_U
 ClientSampleId :
 E29W1

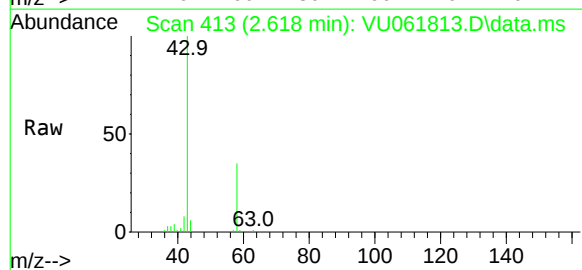

Tgt Ion: 43 Resp: 24857
 Ion Ratio Lower Upper
 43 100
 58 36.3 0.0 69.8

