

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
 Data File : VU061820.D
 Acq On : 18 Nov 2024 18:08
 Operator : MD/SY
 Sample : P4827-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H46W3

Quant Time: Nov 19 00:26:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 00:15:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	167361	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	162143	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	69069	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	37712	3.488	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.800%
7) Chloroethane-d5	1.907	69	35277	3.821	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	2.560	65	17635	3.635	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	4.618	46	109090	47.530	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.060%
24) Chloroform-d	5.052	84	94096	4.378	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.692	65	48600	4.712	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.718	84	189070	4.215	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
36) 1,2-Dichloropropane-d6	6.682	67	61539	4.651	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.000%
41) Toluene-d8	7.891	98	166235	3.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.174	79	18647	3.826	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.600%
46) 2-Hexanone-d5	8.627	63	86489	44.913	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.820%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	48805	4.680	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	58971	4.794	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds						
13) Acetone	2.624	43	32576	22.528	ug/L	97
17) Methyl tert-butyl Ether	3.354	73	77280	3.121	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061820.D
Acq On : 18 Nov 2024 18:08
Operator : MD/SY
Sample : P4827-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46W3

Quant Time: Nov 19 00:26:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 00:15:47 2024
Response via : Initial Calibration

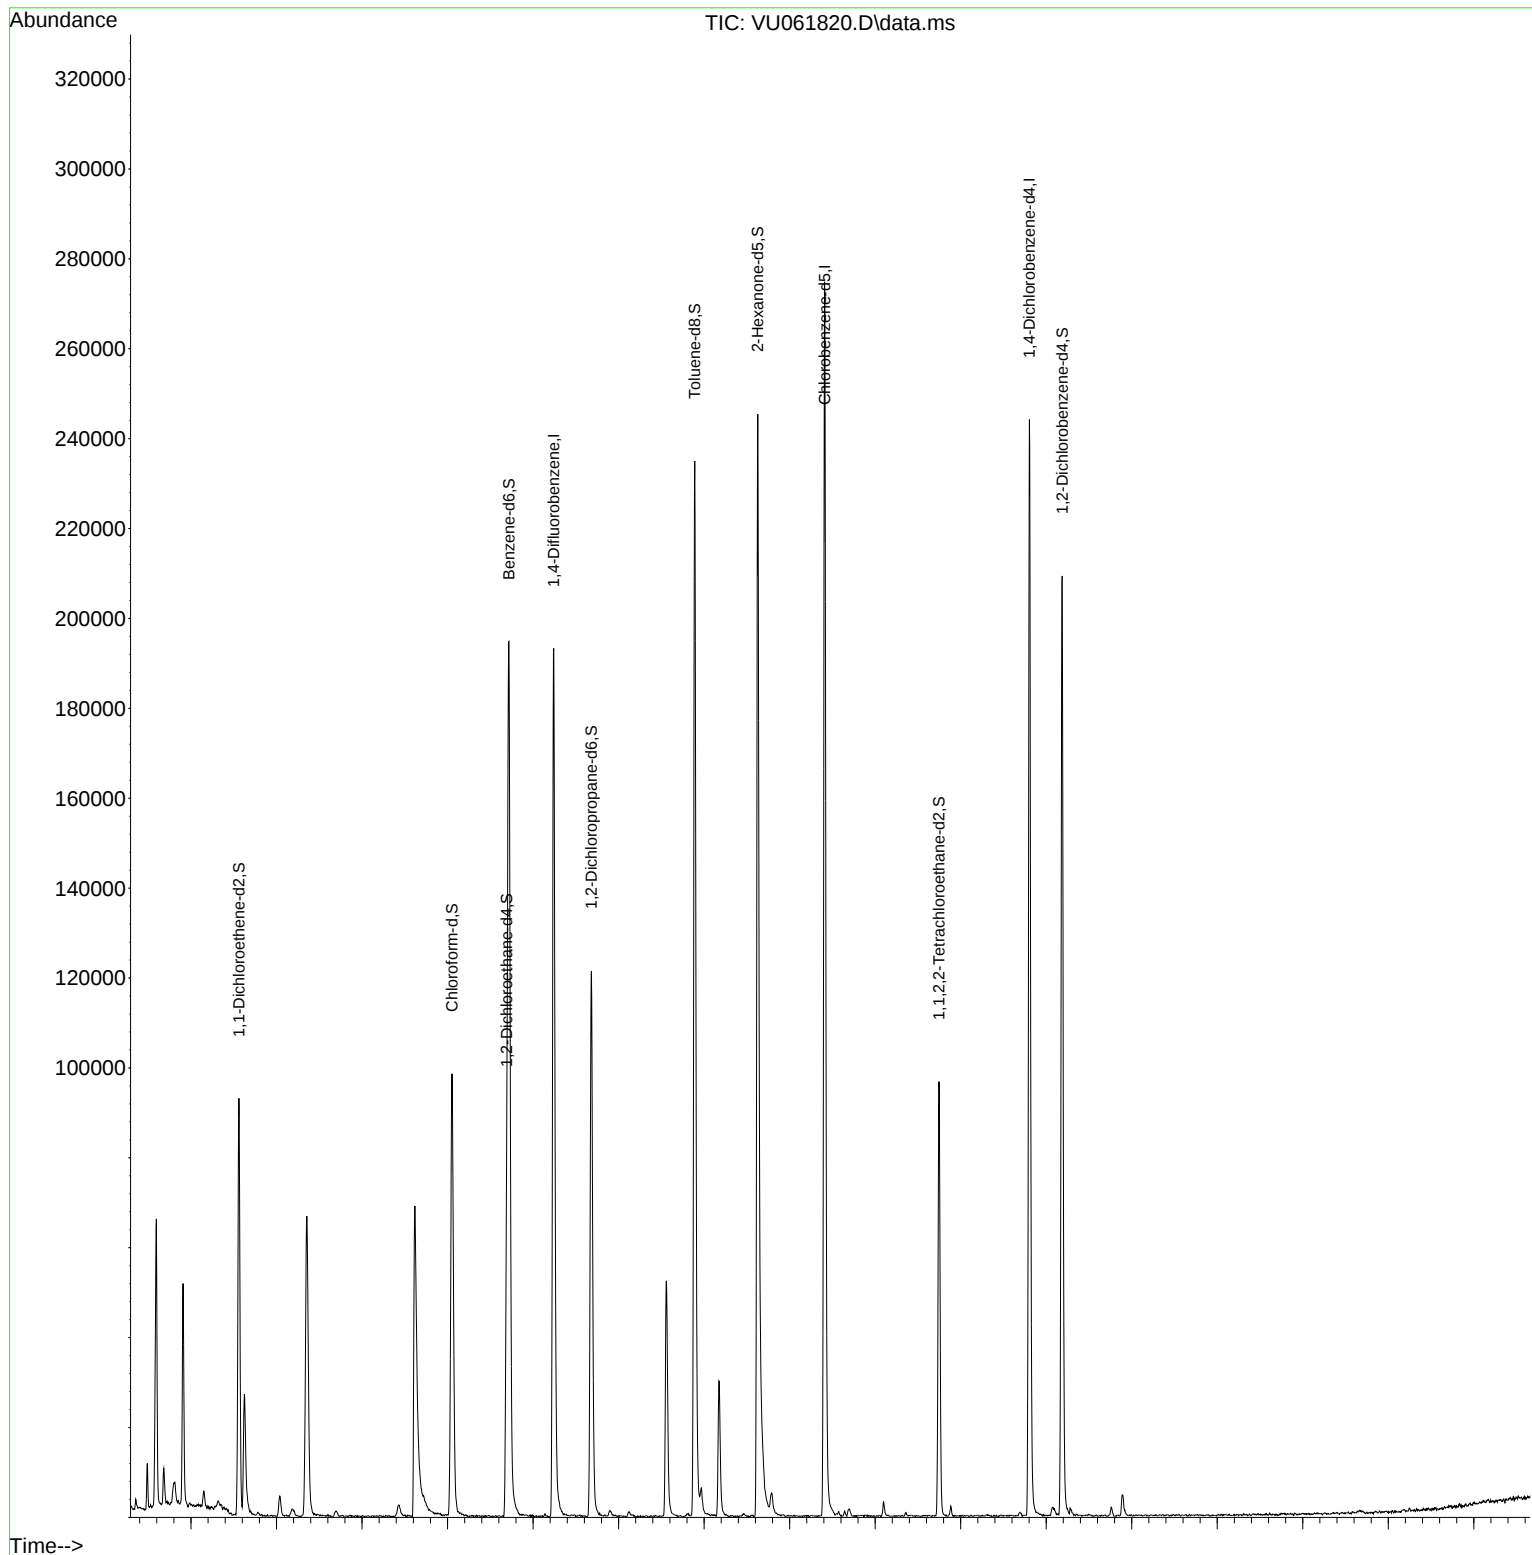

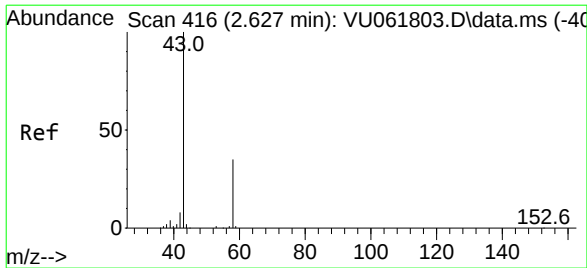

#13

Acetone

Concen: 22.528 ug/L

RT: 2.624 min Scan# 41

Delta R.T. -0.003 min

Lab File: VU061820.D

Acq: 18 Nov 2024 18:08

Instrument :

MSVOA_U

ClientSampleId :





H46W3

Tgt Ion: 43 Resp: 32576

Ion Ratio Lower Upper

43 100

58 36.9 0.0 69.8

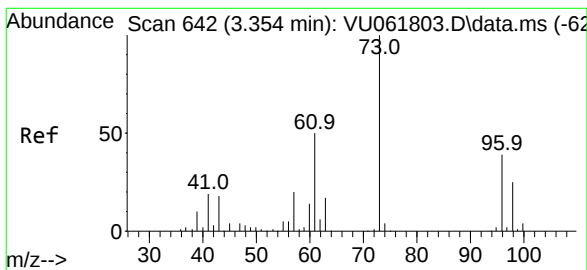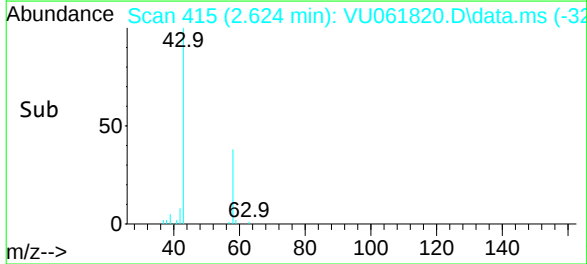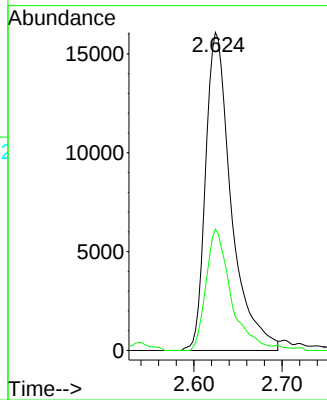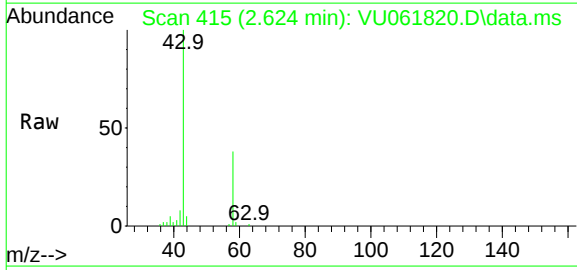

#17

Methyl tert-butyl Ether

Concen: 3.121 ug/L

RT: 3.354 min Scan# 642

Delta R.T. 0.000 min

Lab File: VU061820.D

Acq: 18 Nov 2024 18:08

Tgt Ion: 73 Resp: 77280

Ion Ratio Lower Upper

73 100

43 18.4 14.2 21.4

57 21.0 16.9 25.3

