

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
 Data File : VU061826.D
 Acq On : 18 Nov 2024 21:40
 Operator : MD/SY
 Sample : P4827-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H46W8

Quant Time: Nov 19 03:38:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 03:37:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	175281	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	166176	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	69533	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	36801	3.250	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.000%
7) Chloroethane-d5	1.908	69	35409	3.662	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.200%
11) 1,1-Dichloroethene-d2	2.560	65	17890	3.521	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.400%
20) 2-Butanone-d5	4.612	46	103270	42.962	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.920%
24) Chloroform-d	5.052	84	94963	4.219	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.692	65	48489	4.489	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
32) Benzene-d6	5.718	84	190647	4.147	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.682	67	60318	4.449	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	7.891	98	166520	3.886	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	8.177	79	18837	3.772	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.400%
46) 2-Hexanone-d5	8.624	63	84157	42.642	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.280%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	48267	4.516	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	58593	4.731	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.600%
Target Compounds					Qvalue	
13) Acetone	2.621	43	8208	5.420	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061826.D
Acq On : 18 Nov 2024 21:40
Operator : MD/SY
Sample : P4827-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H46W8


Quant Time: Nov 19 03:38:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 03:37:44 2024
Response via : Initial Calibration

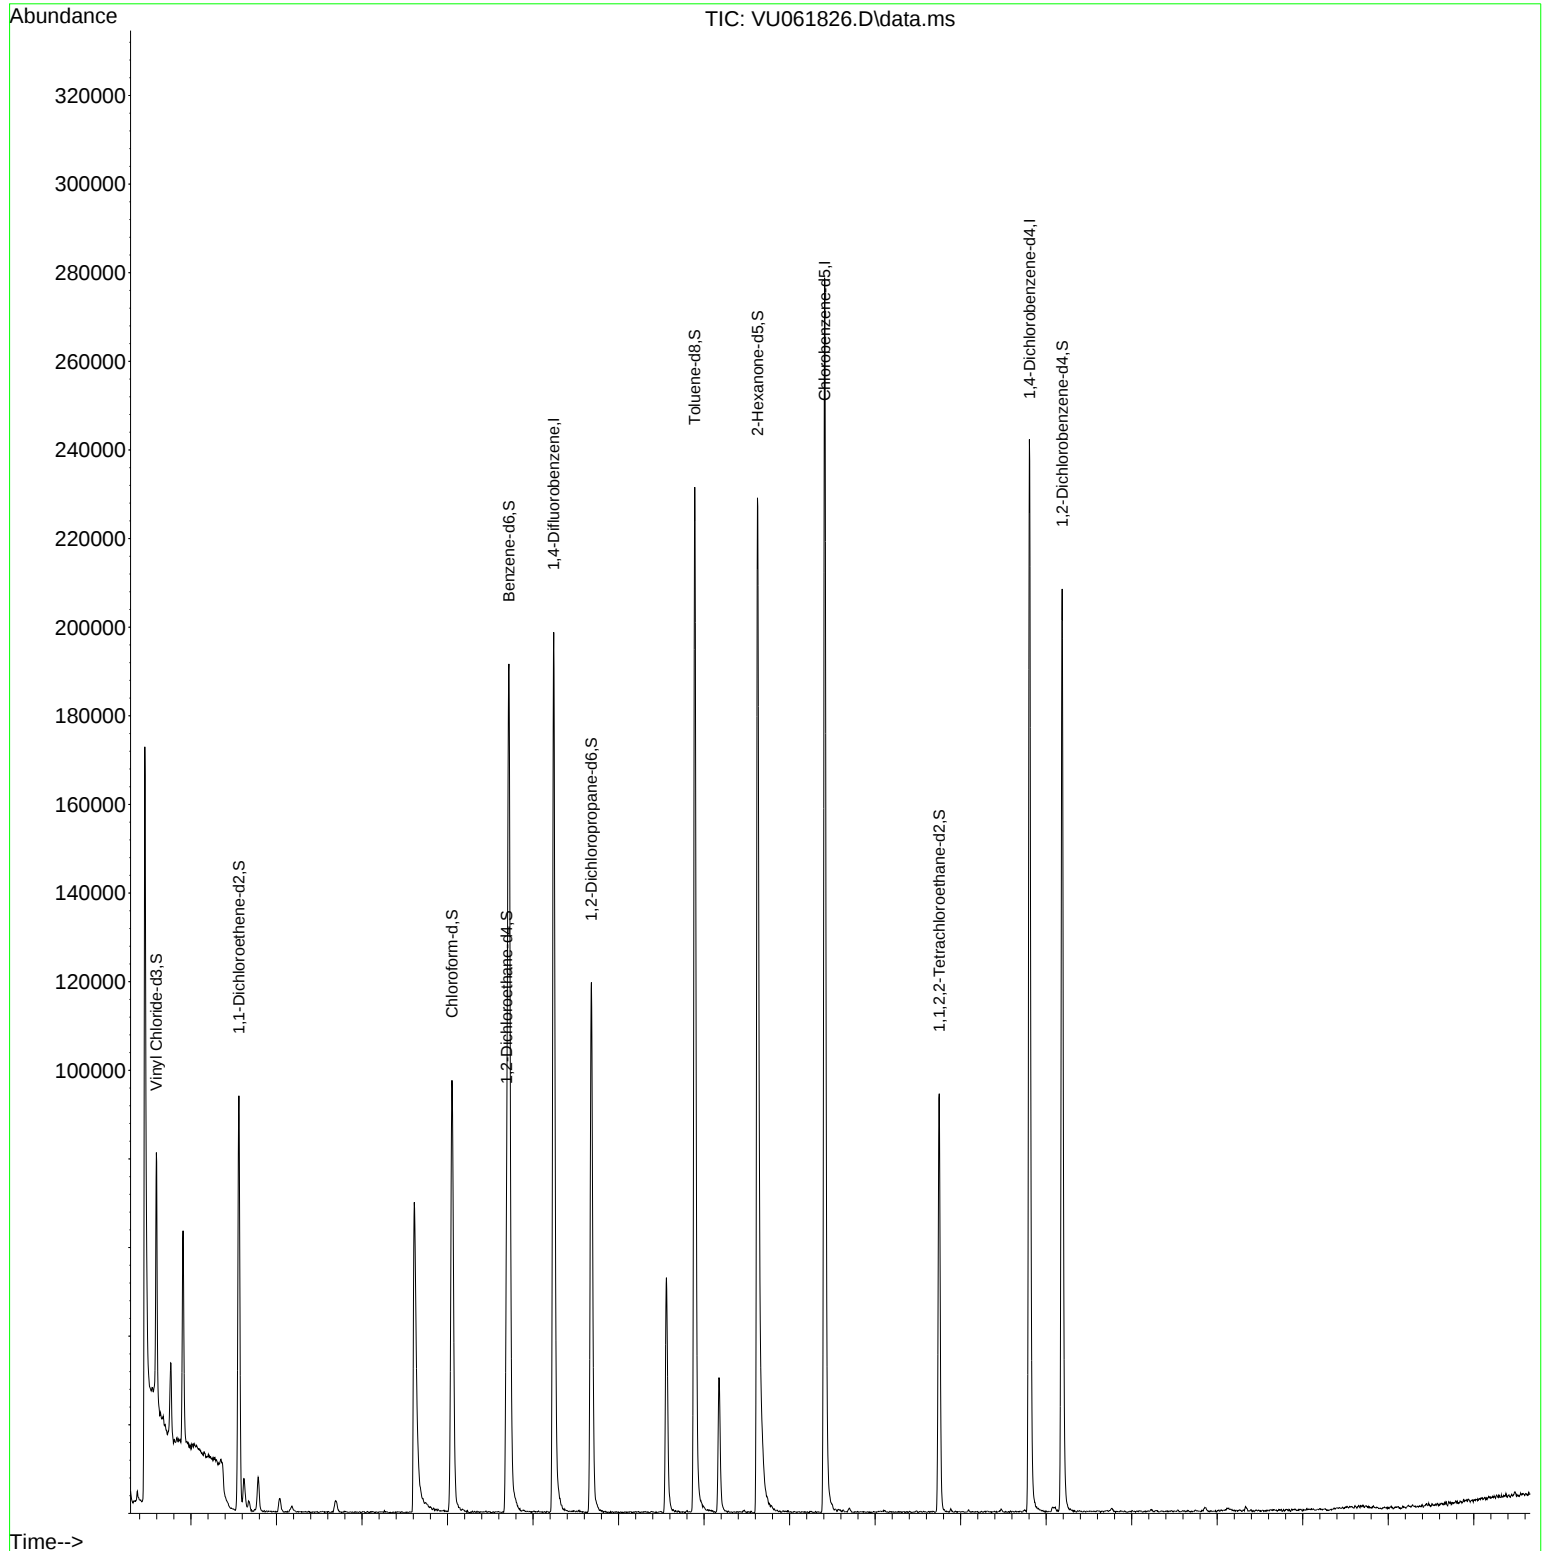

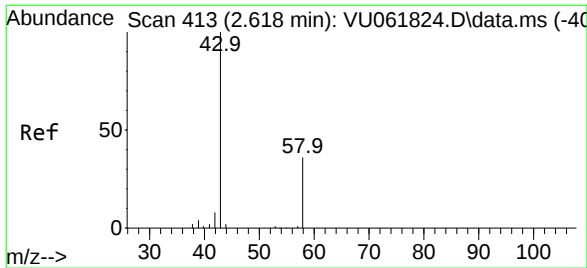

#13
 Acetone
 Concen: 5.420 ug/L
 RT: 2.621 min Scan# 41
 Delta R.T. 0.004 min
 Lab File: VU061826.D
 Acq: 18 Nov 2024 21:40

Instrument :
 MSVOA_U
 ClientSampleId :
 H46W8

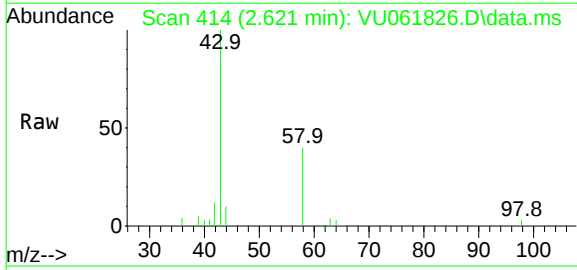

Tgt Ion: 43 Resp: 8208
 Ion Ratio Lower Upper
 43 100
 58 37.5 0.0 69.8

