

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
 Data File : VU061830.D
 Acq On : 18 Nov 2024 23:19
 Operator : MD/SY
 Sample : P4885-15
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3R1

Quant Time: Nov 19 03:39:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 03:37:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	167578	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	213131	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	66817	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	36778	3.397	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.000%
7) Chloroethane-d5	1.907	69	36573	3.957	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.200%
11) 1,1-Dichloroethene-d2	2.560	65	17091	3.518	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.400%
20) 2-Butanone-d5	4.612	46	110309	47.999	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.000%
24) Chloroform-d	5.052	84	94603	4.396	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	5.695	65	48879	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.718	84	190305	3.228	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	64.600%#
36) 1,2-Dichloropropane-d6	6.682	67	59469	3.420	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	68.400%
41) Toluene-d8	7.888	98	166819	3.035	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.800%#
43) trans-1,3-Dichloroprop...	8.174	79	19114	2.984	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	59.600%
46) 2-Hexanone-d5	8.624	63	112729	44.535	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.080%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	47780	3.485	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	69.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	58336	4.902	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds					Qvalue	
13) Acetone	2.618	43	43386	29.965	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061830.D
Acq On : 18 Nov 2024 23:19
Operator : MD/SY
Sample : P4885-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3R1


Quant Time: Nov 19 03:39:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 03:37:44 2024
Response via : Initial Calibration

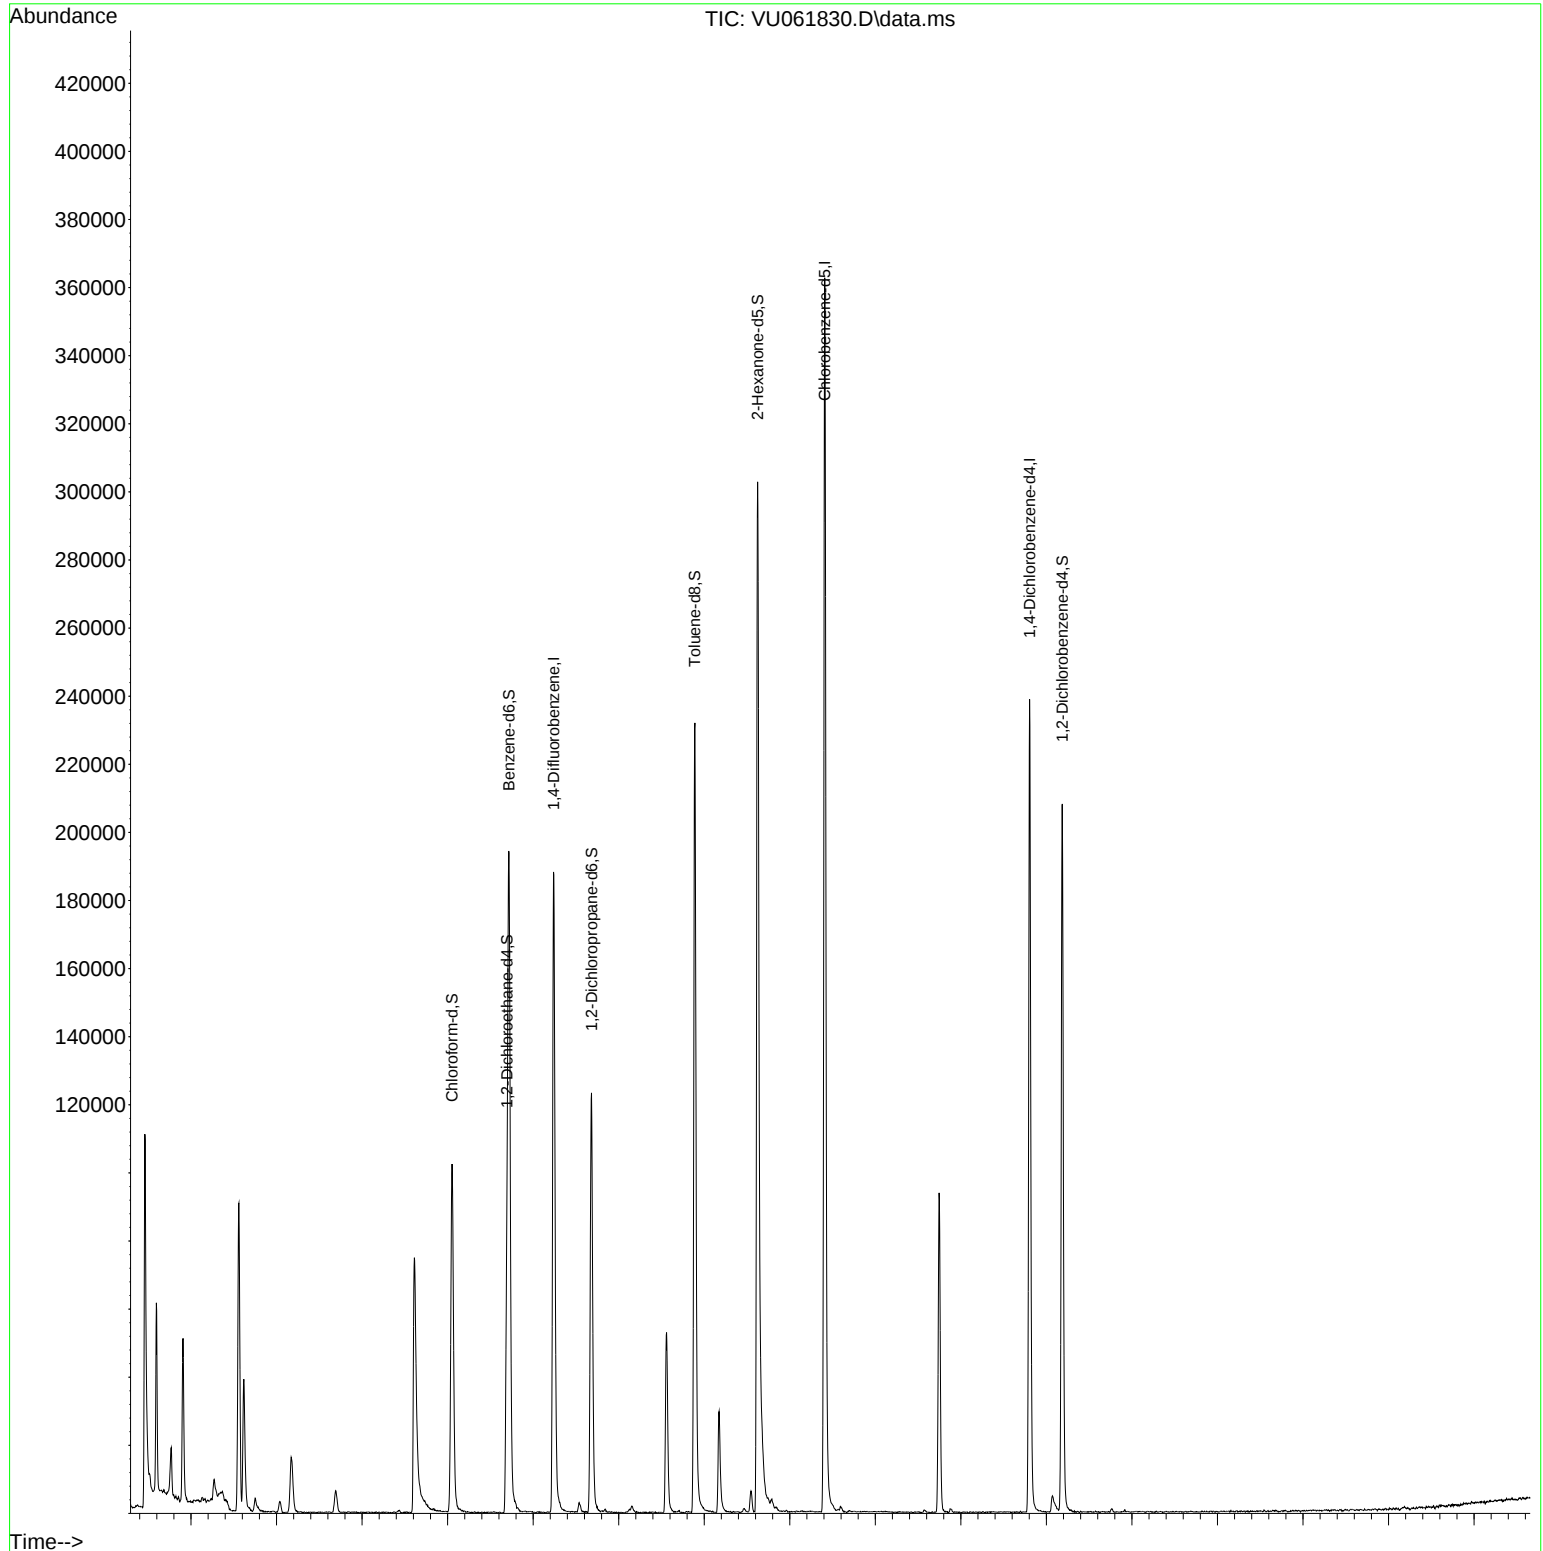

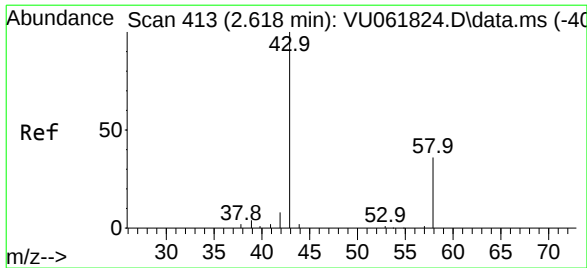

#13
 Acetone
 Concen: 29.965 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU061830.D
 Acq: 18 Nov 2024 23:19

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3R1

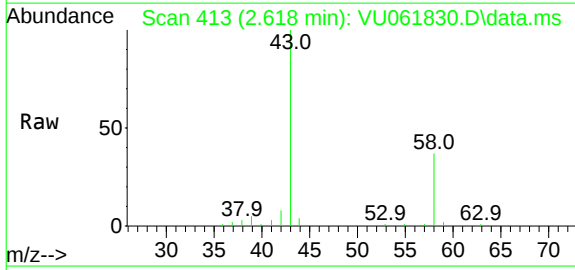

Tgt Ion: 43 Resp: 43386
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 69.8

