

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
 Data File : VU061831.D
 Acq On : 18 Nov 2024 23:44
 Operator : MD/SY
 Sample : P4885-16
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3R2

Quant Time: Nov 19 03:40:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 03:37:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	168751	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	207794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	68171	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	34938	3.204	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.000%
7) Chloroethane-d5	1.907	69	34050	3.658	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.200%
11) 1,1-Dichloroethene-d2	2.560	65	16521	3.377	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	4.611	46	108862	47.040	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.080%
24) Chloroform-d	5.052	84	91380	4.216	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.692	65	48286	4.643	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.718	84	185484	3.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	64.600%#
36) 1,2-Dichloropropane-d6	6.679	67	57093	3.367	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	67.400%
41) Toluene-d8	7.888	98	162128	3.026	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.600%#
43) trans-1,3-Dichloroprop...	8.174	79	17236	2.760	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.200%
46) 2-Hexanone-d5	8.624	63	84574	34.270	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.540%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	69826	5.224	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	55616	4.581	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.600%
Target Compounds					Qvalue	
13) Acetone	2.618	43	40664	27.890	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061831.D
Acq On : 18 Nov 2024 23:44
Operator : MD/SY
Sample : P4885-16
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3R2


Quant Time: Nov 19 03:40:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 03:37:44 2024
Response via : Initial Calibration

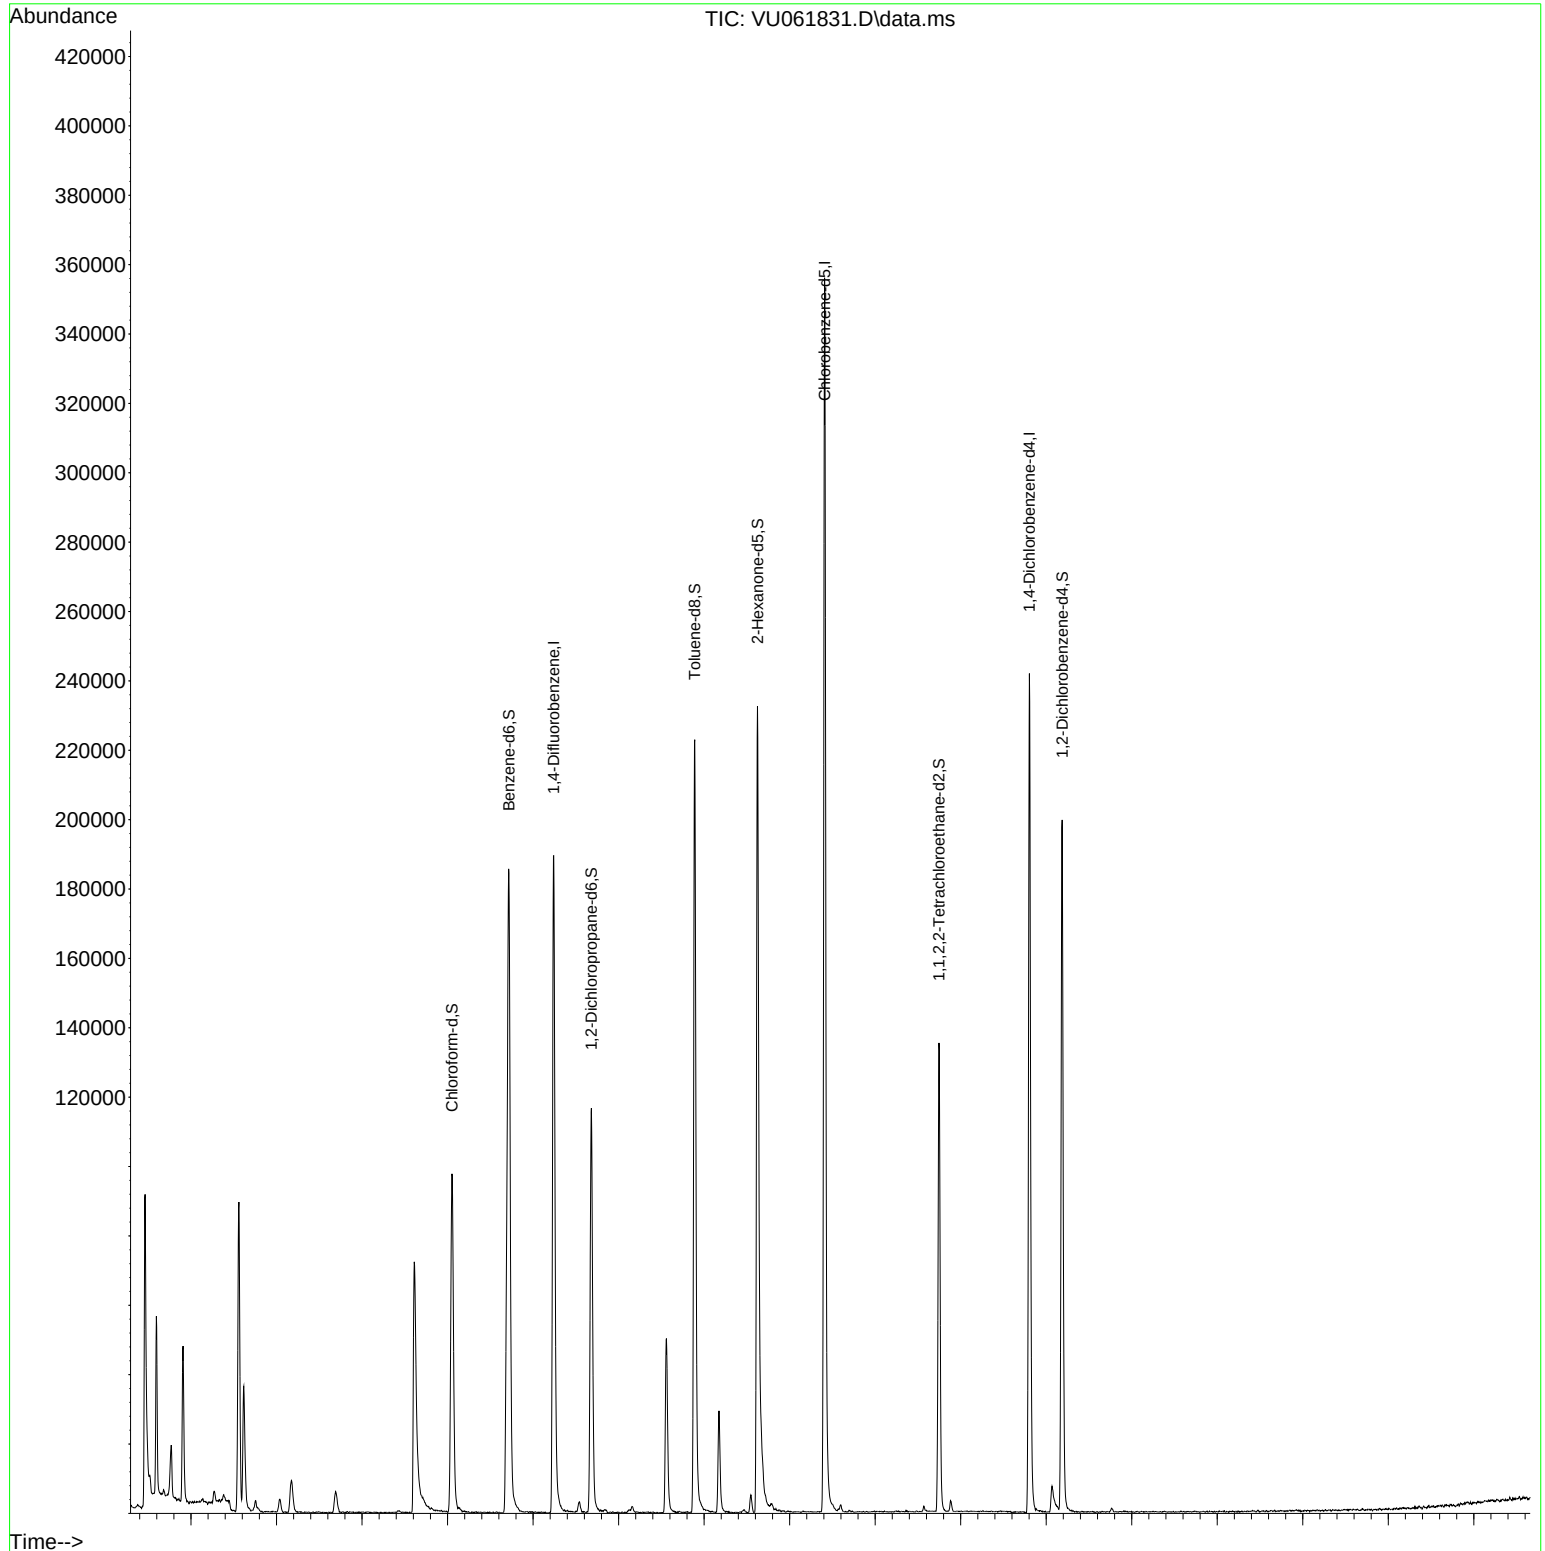

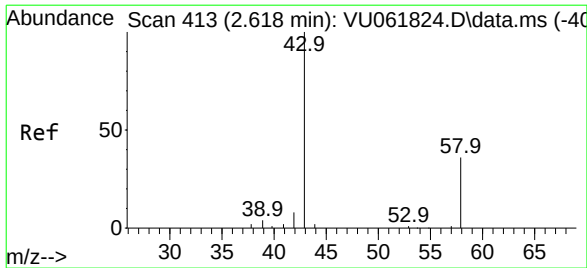

#13
 Acetone
 Concen: 27.890 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU061831.D
 Acq: 18 Nov 2024 23:44

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3R2

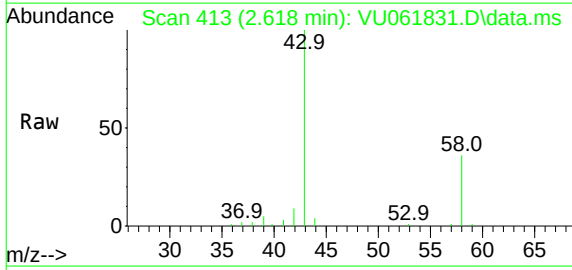

Tgt Ion: 43 Resp: 40664
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 69.8

