
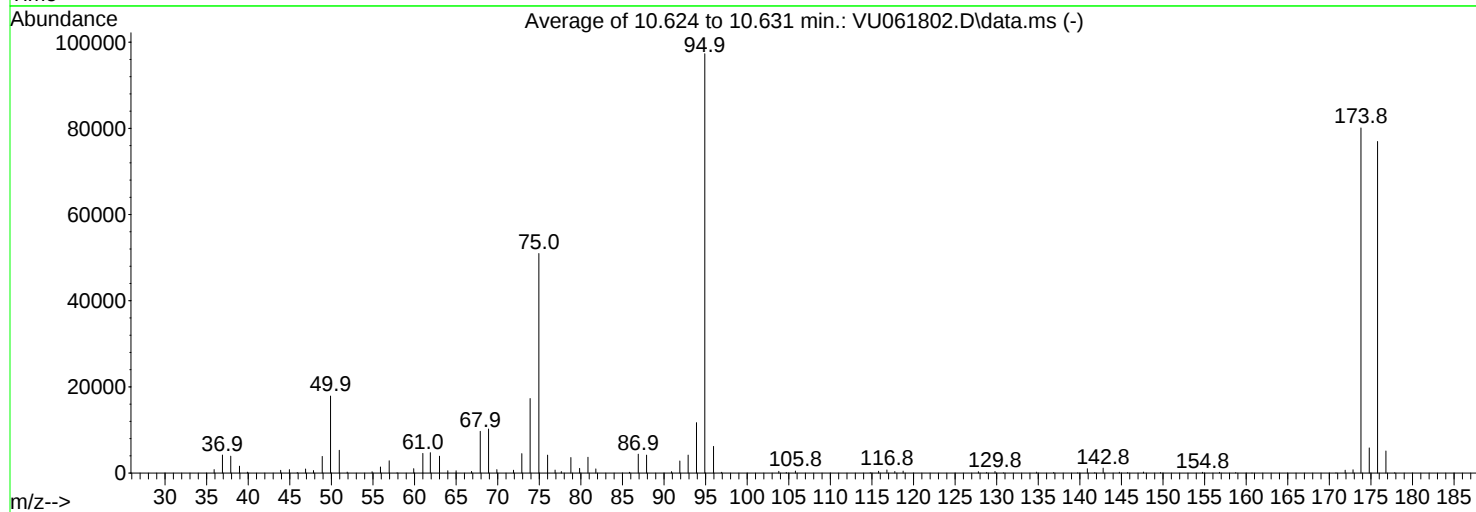


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111824\
Data File : VU061802.D
Acq On : 18 Nov 2024 08:30
Operator : MD/SY
Sample : BFB030
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB030

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 19 03:37:44 2024

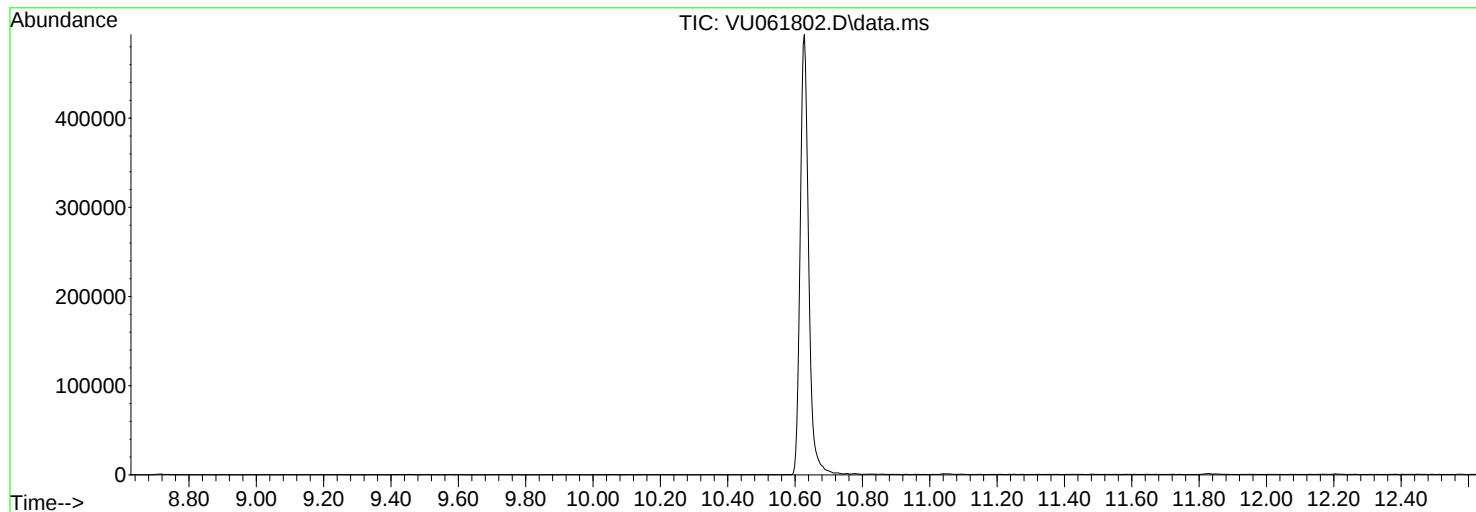

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	17883	PASS
75	95	30	80	52.4	50955	PASS
95	95	100	100	100.0	97323	PASS
96	95	5	9	6.4	6197	PASS
173	174	0.00	2	1.0	770	PASS
174	95	50	120	82.3	80096	PASS
175	174	5	9	7.3	5839	PASS
176	174	95	101	96.1	76960	PASS
177	176	5	9	6.7	5124	PASS

m/z	Abundance
43.90	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	805.0
36.90	4367.0
37.90	4094.0
39.00	1565.0
39.90	228.0
43.90	913.0
45.00	795.0
45.90	142.0
46.90	1013.0
47.90	623.0
48.90	3806.0
49.90	18464.0
51.00	5309.0
51.90	241.0
54.90	358.0
55.90	1352.0
56.90	2967.0
59.90	1037.0
61.00	4766.0
61.90	4936.0
63.00	4096.0
64.00	564.0
65.00	556.0
66.90	418.0
67.90	9762.0
68.90	10133.0
69.90	820.0
71.90	674.0
72.90	4600.0
73.90	17320.0
75.00	51784.0
76.00	4296.0
76.90	724.0
77.60	349.0
78.80	3648.0
79.90	1091.0
80.80	3820.0
81.80	951.0
85.80	194.0
86.90	4619.0
87.90	4375.0
90.90	295.0
91.90	2774.0
92.90	4255.0
93.90	11635.0
94.90	98192.0
95.90	6515.0
97.00	206.0
103.80	377.0
104.70	183.0
105.80	513.0
114.80	126.0
115.80	438.0
116.80	701.0
117.80	348.0
118.80	439.0
127.80	349.0
128.80	166.0
129.80	377.0
130.80	107.0
134.80	212.0
136.90	160.0
140.90	956.0
141.80	113.0
142.80	1154.0
144.70	229.0
145.80	155.0
147.70	265.0
149.70	121.0
154.70	191.0
156.90	152.0
158.80	124.0
170.80	109.0
171.90	649.0
172.80	783.0
173.80	79528.0
174.80	5835.0
175.80	75768.0
176.80	5317.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	851.0
36.90	4288.0
37.90	3996.0
38.90	1612.0
39.90	250.0
43.90	952.0
44.90	826.0
45.90	146.0
46.90	979.0
47.90	596.0
48.90	3949.0
49.90	18336.0
51.00	5447.0
51.90	233.0
54.90	331.0
55.90	1456.0
56.90	2941.0
57.90	100.0
59.90	1085.0
61.00	4654.0
61.90	4833.0
63.00	4019.0
64.00	570.0
65.00	569.0
66.80	397.0
67.90	9977.0
68.90	10632.0
69.90	802.0
71.90	717.0
72.90	4643.0
73.90	17768.0
74.90	52328.0
76.00	4269.0
76.90	708.0
77.60	356.0
78.80	3689.0
79.80	1101.0
80.80	3799.0
81.80	1034.0
85.80	202.0
86.90	4547.0
87.90	4249.0
90.90	342.0
91.90	2914.0
92.90	4265.0
93.90	12035.0
94.90	100208.0
96.00	6369.0
96.90	198.0
103.80	430.0
104.70	157.0
105.80	490.0
114.80	128.0
115.80	445.0
116.80	767.0
117.70	368.0
118.80	462.0
127.80	333.0
128.80	175.0
129.80	384.0
130.80	102.0
134.80	232.0
136.80	148.0
139.80	105.0
140.90	1062.0
141.80	117.0
142.80	1176.0
144.70	206.0
145.70	142.0
147.60	250.0
149.70	134.0
154.80	189.0
156.80	180.0
158.80	148.0
170.80	112.0
171.90	701.0
172.90	774.0
173.80	82488.0
174.80	6076.0
175.80	79280.0
176.80	5237.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
35.90	784.0
36.90	3904.0
37.90	3674.0
38.90	1625.0
39.90	213.0
43.90	901.0
44.90	798.0
45.90	127.0
46.90	842.0
47.80	553.0
48.90	3845.0
49.90	16848.0
50.90	5117.0
51.90	222.0
54.90	252.0
55.90	1427.0
57.00	2639.0
57.90	106.0
59.90	953.0
61.00	4276.0
61.90	4442.0
63.00	3656.0
64.00	517.0
65.00	504.0
66.80	323.0
67.90	9358.0
68.90	9937.0
69.90	803.0
71.90	622.0
72.90	4314.0
73.90	16824.0
74.90	48752.0
76.00	3944.0
76.90	677.0
77.70	333.0
78.80	3489.0
79.80	1078.0
80.90	3423.0
81.80	940.0
85.90	177.0
86.90	4003.0
87.90	3874.0
90.90	386.0
91.90	2748.0
92.90	4017.0
93.90	11443.0
94.90	93568.0
96.00	5706.0
96.80	173.0
103.80	425.0
104.70	112.0
105.80	405.0
115.80	386.0
116.80	742.0
117.70	410.0
118.70	501.0
127.80	310.0
128.80	173.0
129.80	368.0
134.80	240.0
136.80	128.0
139.70	103.0
140.90	1035.0
141.80	119.0
142.80	1108.0
144.80	173.0
145.70	115.0
147.70	213.0
149.70	105.0
154.80	197.0
156.70	225.0
158.70	140.0
160.70	114.0
171.90	672.0
172.90	753.0
173.80	78272.0
174.80	5606.0
175.80	75832.0
176.80	4819.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030