
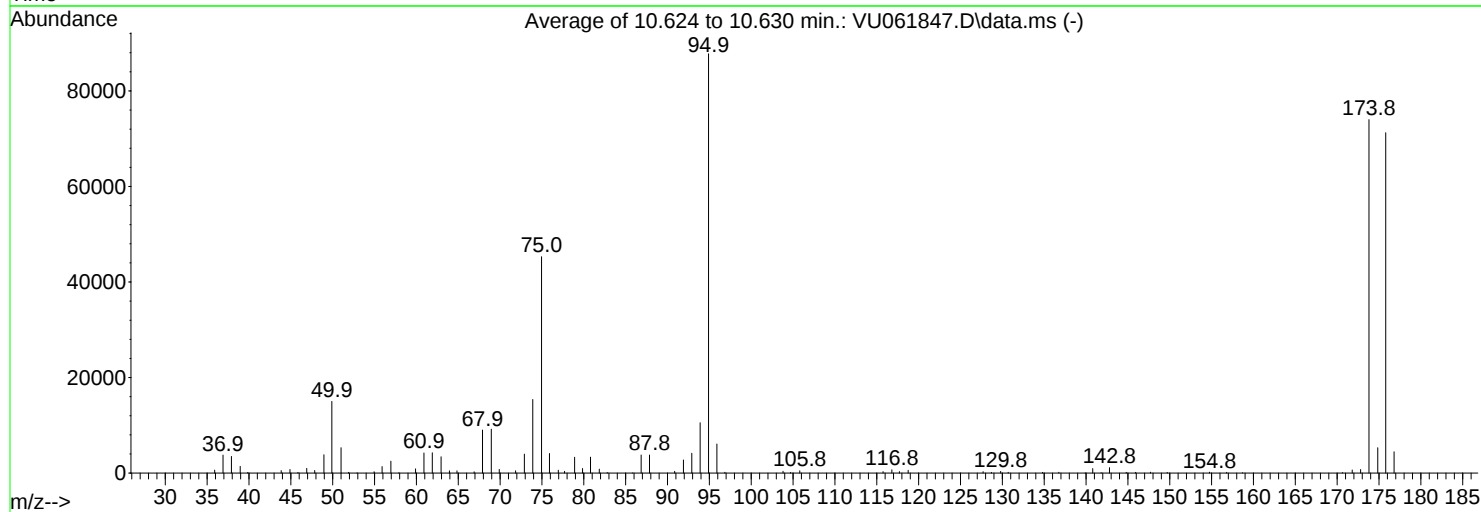


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111924\
Data File : VU061847.D
Acq On : 19 Nov 2024 08:42
Operator : MD/SY
Sample : BFB031
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB031

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 20 01:26:01 2024

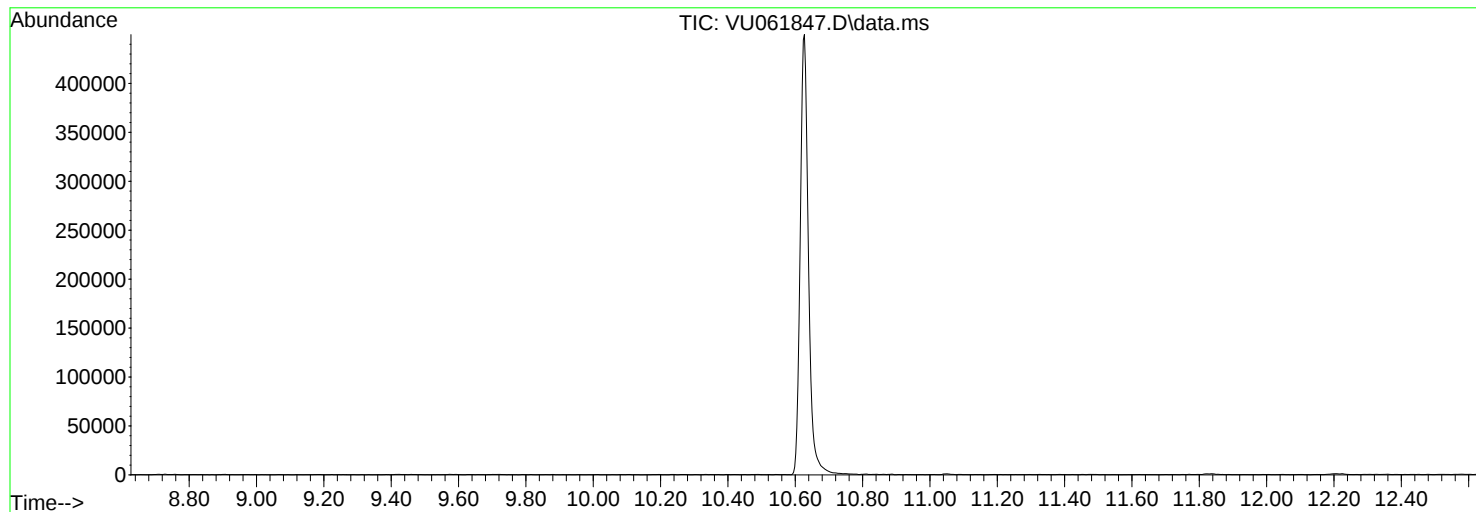

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	15001	PASS
75	95	30	80	51.6	45299	PASS
95	95	100	100	100.0	87789	PASS
96	95	5	9	6.9	6090	PASS
173	174	0.00	2	1.0	751	PASS
174	95	50	120	84.3	73997	PASS
175	174	5	9	7.2	5306	PASS
176	174	95	101	96.3	71253	PASS
177	176	5	9	6.3	4466	PASS

m/z	Abundance
43.80	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	682.0
36.90	3914.0
37.90	3607.0
38.90	1404.0
39.80	118.0
43.90	807.0
44.90	852.0
45.80	155.0
46.90	1040.0
47.90	534.0
48.90	4092.0
49.90	15614.0
51.00	5472.0
51.90	148.0
54.90	358.0
55.90	1425.0
57.00	2680.0
57.90	110.0
59.90	955.0
60.90	4333.0
61.90	4229.0
63.00	3446.0
64.00	545.0
64.90	458.0
66.90	248.0
67.90	9358.0
68.90	9359.0
69.90	806.0
71.80	501.0
72.90	4076.0
73.90	15839.0
74.90	46480.0
75.90	4260.0
76.90	563.0
77.70	377.0
78.90	3510.0
79.80	999.0
80.80	3431.0
81.90	883.0
82.80	105.0
85.80	129.0
86.80	3892.0
87.90	4054.0
90.90	367.0
91.90	2776.0
92.90	4097.0
93.90	11035.0
94.90	89368.0
95.90	6194.0
96.90	198.0
103.80	390.0
104.70	144.0
105.80	519.0
115.70	328.0
116.80	685.0
117.70	304.0
118.80	606.0
127.70	343.0
128.70	175.0
129.80	345.0
130.70	151.0
134.80	181.0
136.80	188.0
140.80	973.0
142.80	1130.0
144.80	188.0
145.90	147.0
147.70	177.0
149.70	123.0
154.70	205.0
156.80	136.0
158.70	134.0
170.70	103.0
171.70	667.0
172.80	855.0
173.80	74904.0
174.80	5383.0
175.80	70408.0
176.80	4684.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	641.0
36.90	3856.0
37.90	3596.0
38.90	1423.0
39.90	131.0
43.90	785.0
44.90	770.0
45.90	145.0
46.90	1024.0
47.90	568.0
48.90	3984.0
49.90	15485.0
51.00	5486.0
51.90	155.0
52.90	101.0
54.90	298.0
55.90	1406.0
56.90	2542.0
59.90	915.0
60.90	4327.0
61.90	4382.0
63.00	3508.0
63.90	454.0
64.90	503.0
66.90	290.0
67.90	9318.0
69.00	9488.0
69.90	782.0
71.90	500.0
72.90	4079.0
73.90	15840.0
75.00	46616.0
75.90	4213.0
76.90	644.0
77.70	382.0
78.90	3406.0
79.80	975.0
80.80	3436.0
81.90	853.0
82.80	124.0
86.80	3886.0
87.90	3890.0
90.90	391.0
91.90	2838.0
92.90	4320.0
93.90	10740.0
94.90	90488.0
95.90	6338.0
96.90	180.0
103.80	395.0
104.70	140.0
105.80	504.0
115.70	313.0
116.80	714.0
117.70	328.0
118.80	618.0
127.70	313.0
128.70	155.0
129.80	372.0
130.70	179.0
134.80	146.0
136.80	173.0
140.80	984.0
141.80	124.0
142.80	1166.0
144.80	172.0
145.90	156.0
147.70	203.0
149.70	153.0
154.80	198.0
156.80	151.0
158.70	115.0
170.70	114.0
171.80	666.0
172.80	763.0
173.80	76400.0
174.90	5487.0
175.80	73496.0
176.80	4615.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	561.0
36.90	3547.0
37.90	3273.0
39.00	1408.0
39.90	141.0
43.90	709.0
44.90	650.0
45.90	126.0
46.90	905.0
47.80	533.0
49.00	3447.0
49.90	13904.0
51.00	4980.0
51.90	158.0
55.00	224.0
55.90	1280.0
56.90	2261.0
59.90	784.0
60.90	3985.0
61.90	4149.0
62.90	3304.0
63.90	407.0
64.80	474.0
66.90	278.0
67.90	8364.0
69.00	8735.0
69.90	738.0
71.90	461.0
72.90	3770.0
73.90	14555.0
75.00	42800.0
75.90	3815.0
77.00	642.0
77.70	367.0
78.90	3046.0
79.90	884.0
80.80	3153.0
81.80	755.0
82.80	126.0
86.90	3587.0
87.80	3440.0
90.80	349.0
91.90	2632.0
92.90	4029.0
93.90	9858.0
94.90	83512.0
95.90	5737.0
96.80	151.0
103.80	356.0
104.70	112.0
105.80	420.0
115.80	300.0
116.80	691.0
117.70	324.0
118.70	540.0
127.70	251.0
128.70	128.0
129.80	366.0
130.70	168.0
134.80	135.0
136.70	168.0
139.90	100.0
140.80	886.0
141.80	117.0
142.80	1102.0
144.80	121.0
145.90	140.0
147.70	207.0
149.70	144.0
154.80	172.0
156.80	159.0
170.60	104.0
171.90	621.0
172.80	634.0
173.80	70688.0
174.90	5048.0
175.80	69856.0
176.80	4100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031