

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051983.D
 Acq On : 20 Nov 2022 19:06
 Operator : JC/MD
 Sample : N5710-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY7

Quant Time: Nov 21 01:03:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 18 00:53:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	437873	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	443149	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	159816	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	81372	37.854	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.700%
7) Chloroethane-d5	1.906	69	93313	43.325	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.660%
11) 1,1-Dichloroethene-d2	2.568	63	152418	39.539	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.080%
21) 2-Butanone-d5	4.616	46	249551	102.091	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.090%
24) Chloroform-d	5.060	84	251922	46.750	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.500%
26) 1,2-Dichloroethane-d4	5.700	65	158539	48.062	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.120%
32) Benzene-d6	5.726	84	432296	46.786	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.580%
36) 1,2-Dichloropropane-d6	6.687	67	170681	49.626	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.260%
41) Toluene-d8	7.896	98	320624	42.276	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.560%
43) trans-1,3-Dichloroprop...	8.176	79	55510	40.520	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.040%
47) 2-Hexanone-d5	8.629	63	169677	97.072	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.070%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	315434	47.123	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.240%
66) 1,2-Dichlorobenzene-d4	12.192	152	153850	54.703	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.604	62	19792	5.345	ug/L	# 74
12) 1,1-Dichloroethene	2.578	96	96774	37.086	ug/L	98
14) Carbon disulfide	2.793	76	5857	0.810	ug/L	98
19) 1,1-Dichloroethane	3.870	63	20131	3.517	ug/L	96
20) cis-1,2-Dichloroethene	4.665	96	229601	69.959	ug/L	99
30) 1,1,1-Trichloroethane	5.314	97	25079	5.598	ug/L	97
34) Trichloroethene	6.539	95	300824	99.613	ug/L	99
46) Tetrachloroethene	8.552	164	434495	180.155	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051983.D
Acq On : 20 Nov 2022 19:06
Operator : JC/MD
Sample : N5710-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KY7

Quant Time: Nov 21 01:03:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 18 00:53:49 2022
Response via : Initial Calibration




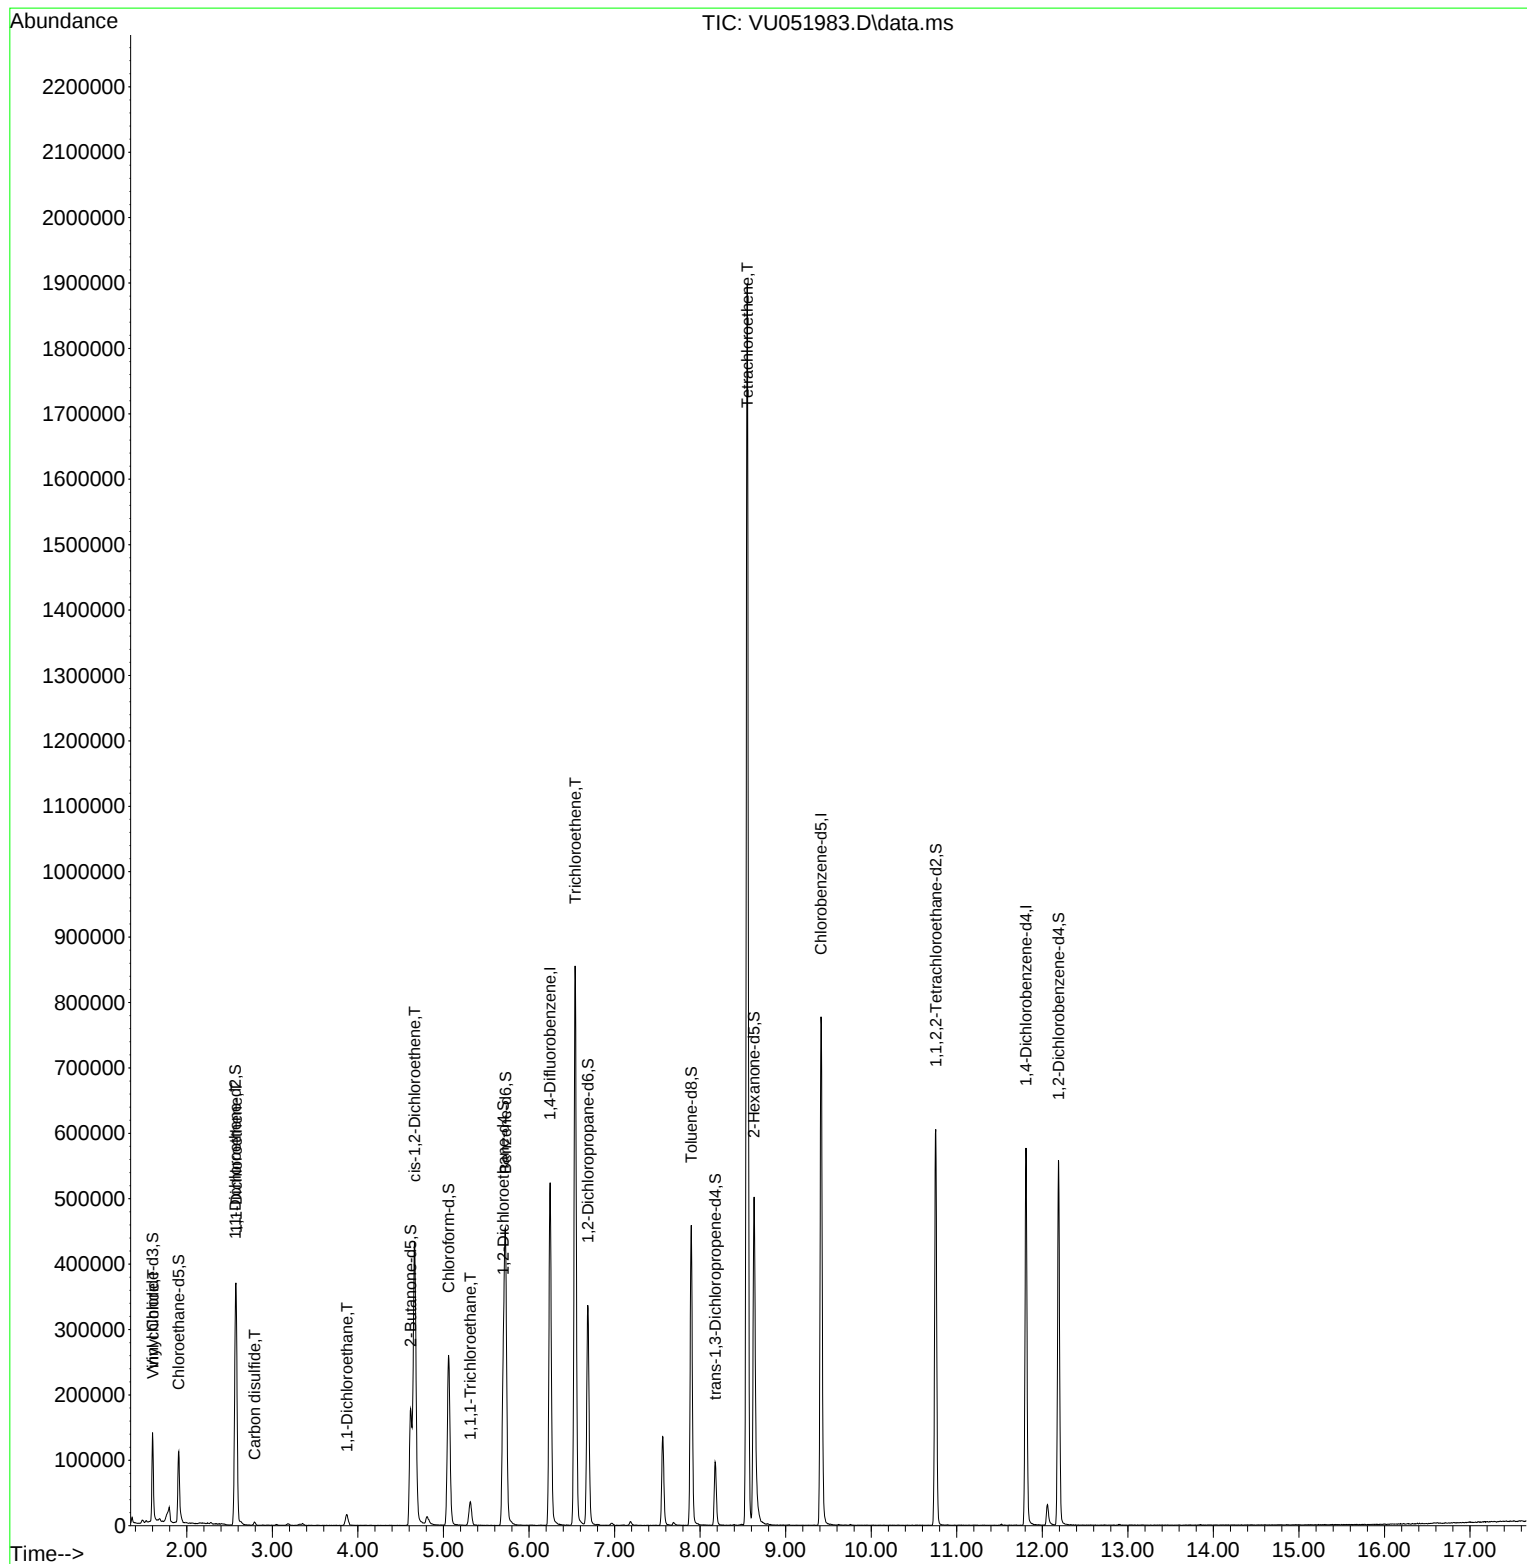


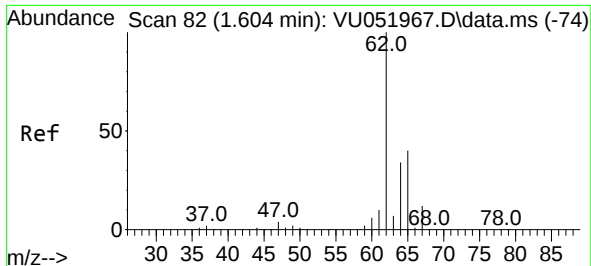

#5
 Vinyl chloride
 Concen: 5.345 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU051983.D
 Acq: 20 Nov 2022 19:06




Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY7


Tgt Ion: 62 Resp: 19792
 Ion Ratio Lower Upper
 62 100
 64 49.7 24.3 45.1#

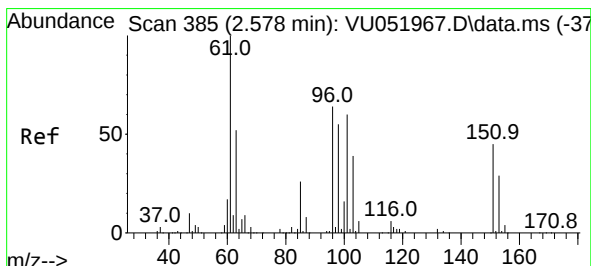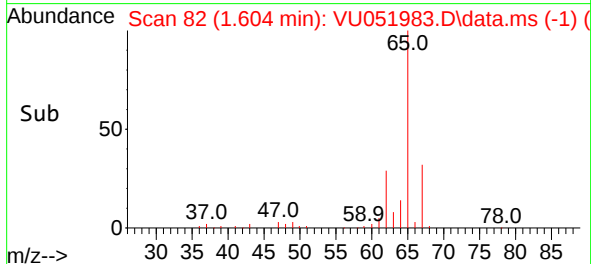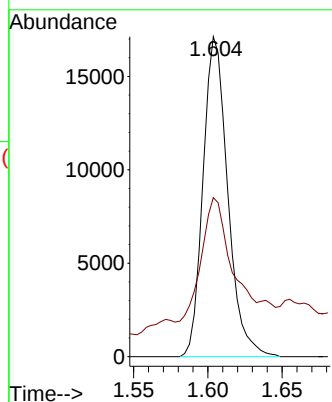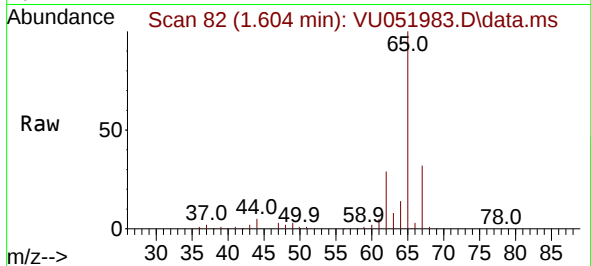

#12
 1,1-Dichloroethene
 Concen: 37.086 ug/L
 RT: 2.578 min Scan# 385
 Delta R.T. 0.003 min
 Lab File: VU051983.D
 Acq: 20 Nov 2022 19:06

Tgt Ion: 96 Resp: 96774
 Ion Ratio Lower Upper
 96 100
 61 161.0 110.7 205.5
 63 99.7 68.6 127.4


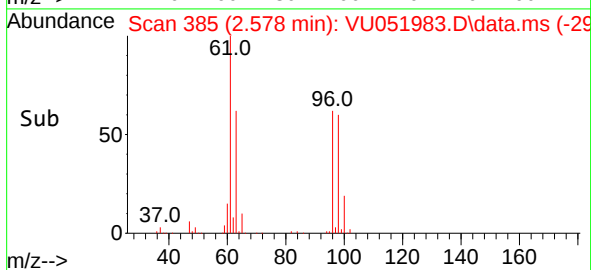
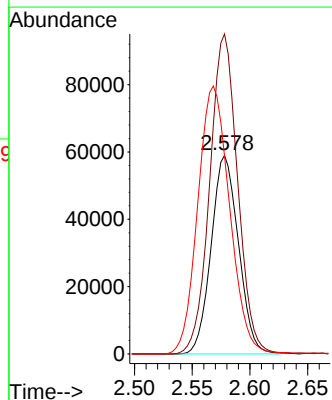
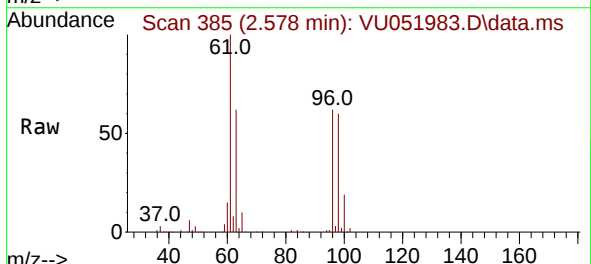


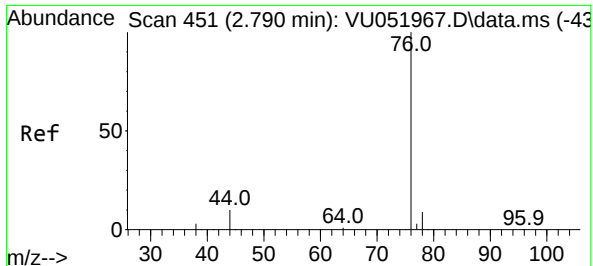

#14
Carbon disulfide
Concen: 0.810 ug/L
RT: 2.793 min Scan# 41
Delta R.T. 0.003 min
Lab File: VU051983.D
Acq: 20 Nov 2022 19:06




Instrument :
MSVOA_U
ClientSampleId :
C0KY7


Tgt Ion: 76 Resp: 5857
Ion Ratio Lower Upper
76 100
78 9.9 7.4 11.0

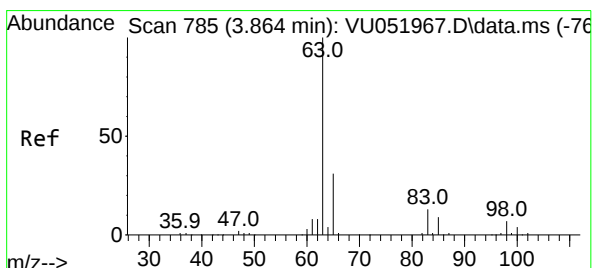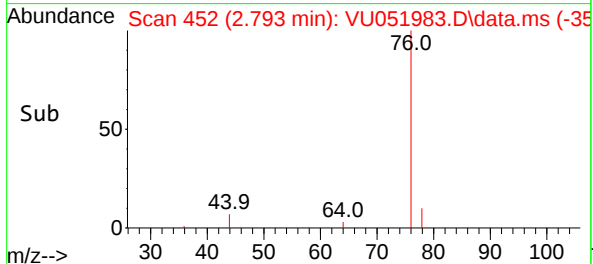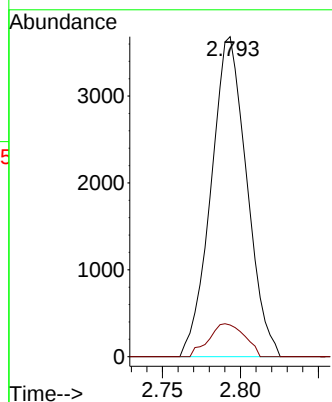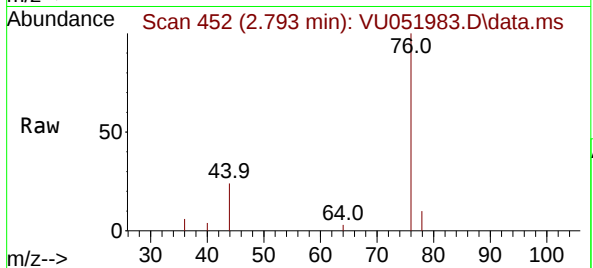

#19
1,1-Dichloroethane
Concen: 3.517 ug/L
RT: 3.870 min Scan# 787
Delta R.T. 0.006 min
Lab File: VU051983.D
Acq: 20 Nov 2022 19:06

Tgt Ion: 63 Resp: 20131
Ion Ratio Lower Upper
63 100
65 30.5 22.2 41.2
83 10.9 9.6 17.8

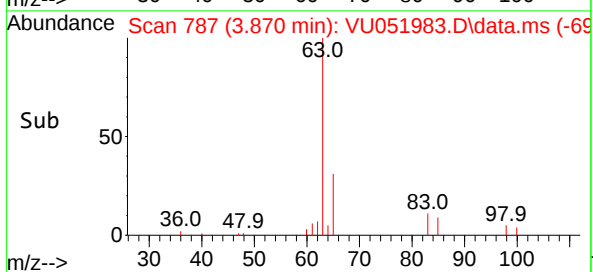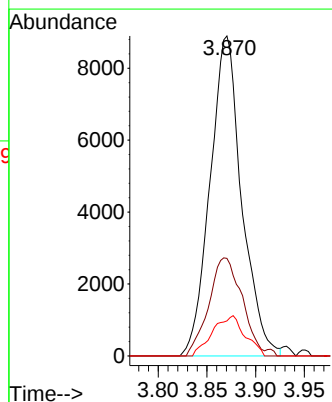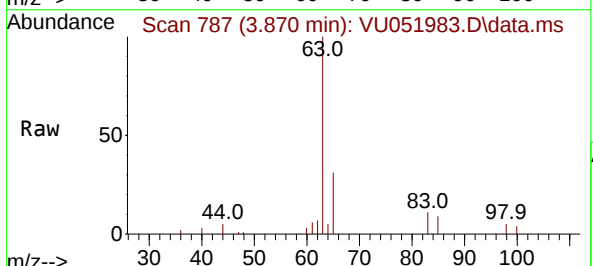




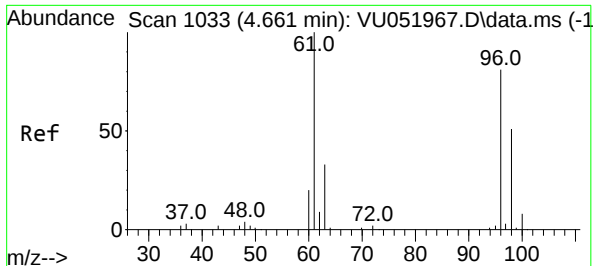


#20
 cis-1,2-Dichloroethene
 Concen: 69.959 ug/L
 RT: 4.665 min Scan# 1033
 Delta R.T. -0.000 min
 Lab File: VU051983.D
 Acq: 20 Nov 2022 19:06

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY7

Tgt Ion: 96 Resp: 229601




Ion	Ratio	Lower	Upper
96	100		
61	124.0	86.0	159.8
68	0.0	0.0	0.0

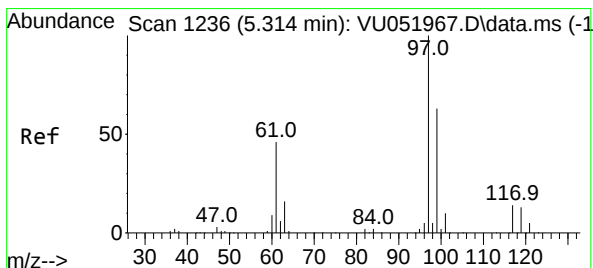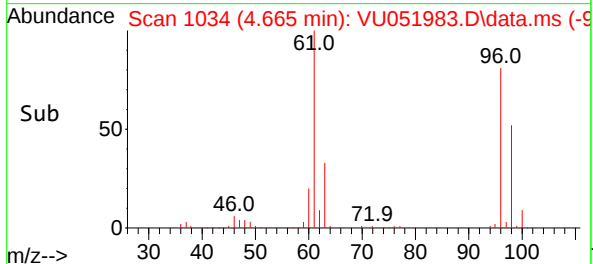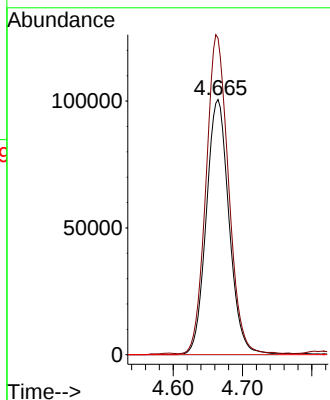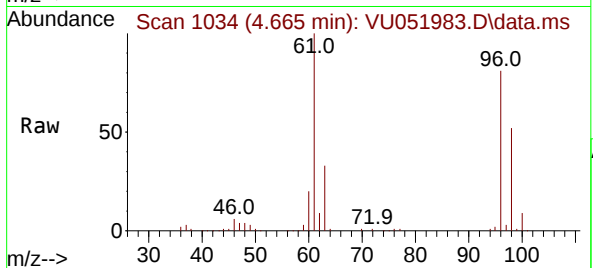


#30
 1,1,1-Trichloroethane
 Concen: 5.598 ug/L
 RT: 5.314 min Scan# 1236
 Delta R.T. -0.000 min
 Lab File: VU051983.D
 Acq: 20 Nov 2022 19:06

Tgt Ion: 97 Resp: 25079

Ion	Ratio	Lower	Upper
97	100		
99	64.4	51.2	76.8
61	50.3	37.4	56.2

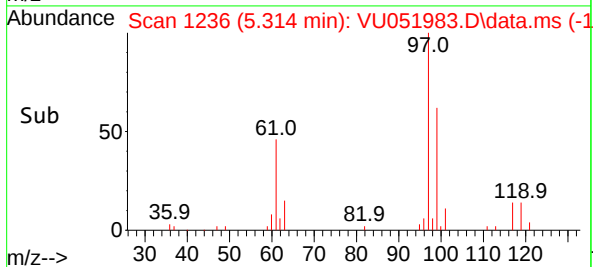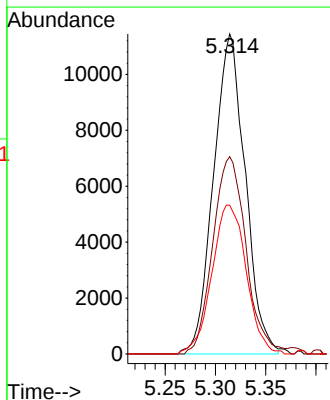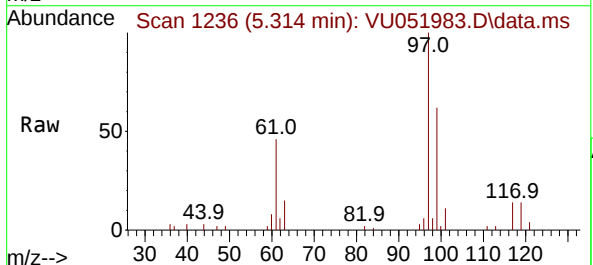

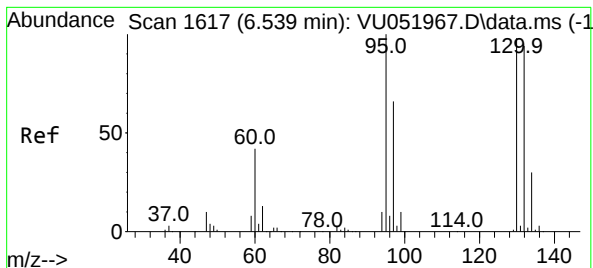

#34

Trichloroethene

Concen: 99.613 ug/L

RT: 6.539 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU051983.D

Acq: 20 Nov 2022 19:06

Instrument :

MSVOA_U

ClientSampleId :

C0KY7

Tgt Ion: 95 Resp: 300824





Ion Ratio Lower Upper

95 100

97 65.2 45.8 85.0

132 95.2 65.3 121.3

130 99.9 69.3 128.7

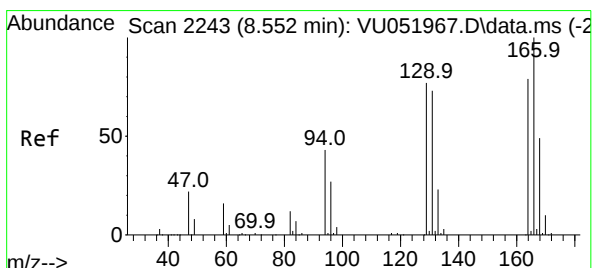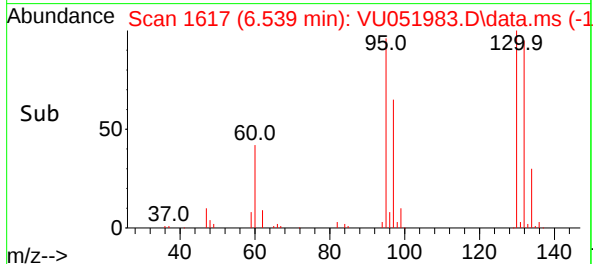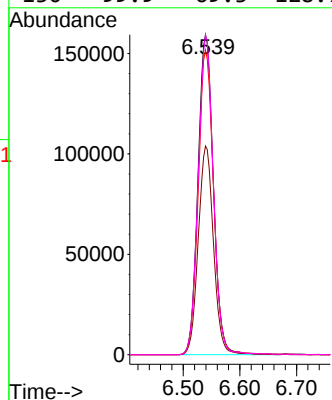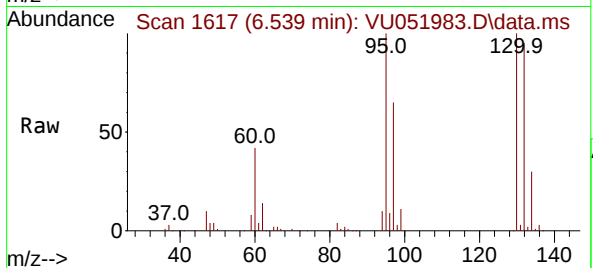

#46

Tetrachloroethene

Concen: 180.155 ug/L

RT: 8.552 min Scan# 2243

Delta R.T. -0.000 min

Lab File: VU051983.D

Acq: 20 Nov 2022 19:06

Tgt Ion:164 Resp: 434495

Ion Ratio Lower Upper

164 100

129 97.2 68.5 127.1

131 94.2 66.6 123.8

166 128.7 91.9 170.7

