

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051968.D
 Acq On : 20 Nov 2022 12:31
 Operator : JC/MD
 Sample : VU1120WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M

Title : VOC Analysis

Signal : TIC: VU051968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	95	rBV	123996	147158	10.67%	1.284%
2	1.903	167	175	199	rVB	120638	183802	13.32%	1.604%
3	2.565	369	381	398	rBV	197606	322159	23.35%	2.812%
4	2.755	436	440	441	rBV2	365	256	0.02%	0.002%
5	2.900	479	485	489	rBV2	537	517	0.04%	0.005%
6	2.951	497	501	504	rBV2	421	309	0.02%	0.003%
7	2.986	509	512	517	rBV2	379	429	0.03%	0.004%
8	3.047	521	531	538	rBV4	3176	5162	0.37%	0.045%
9	3.182	560	573	589	rBV2	8190	17793	1.29%	0.155%
10	3.263	595	598	601	rBV	190	187	0.01%	0.002%
11	3.298	607	609	613	rBV2	167	116	0.01%	0.001%
12	3.353	617	626	629	rBV2	440	501	0.04%	0.004%
13	3.375	629	633	637	rBV2	244	202	0.01%	0.002%
14	3.424	643	648	650	rBV2	238	217	0.02%	0.002%
15	3.459	656	659	661	rVB	158	82	0.01%	0.001%
16	3.472	661	663	666	rBV	279	188	0.01%	0.002%
17	3.520	673	678	681	rBV	193	205	0.01%	0.002%
18	3.562	685	691	694	rBV	206	196	0.01%	0.002%
19	3.646	713	717	721	rBV2	320	248	0.02%	0.002%
20	3.797	761	764	767	rBV2	250	158	0.01%	0.001%
21	3.813	767	769	772	rBV	130	82	0.01%	0.001%
22	3.867	783	786	788	rBV	212	142	0.01%	0.001%
23	3.945	806	810	812	rBV2	195	152	0.01%	0.001%
24	3.961	812	815	821	rVB2	149	148	0.01%	0.001%
25	3.999	825	827	831	rBV	201	187	0.01%	0.002%
26	4.070	846	849	852	rBV	211	139	0.01%	0.001%
27	4.089	852	855	858	rBV	185	147	0.01%	0.001%
28	4.137	867	870	872	rBV2	128	76	0.01%	0.001%
29	4.192	884	887	890	rBV2	232	182	0.01%	0.002%
30	4.263	905	909	910	rBV	129	92	0.01%	0.001%
31	4.391	947	949	953	rVB	233	115	0.01%	0.001%
32	4.414	953	956	958	rBV	311	212	0.02%	0.002%
33	4.472	966	974	977	rBV2	252	277	0.02%	0.002%
34	4.491	977	980	982	rBV2	204	150	0.01%	0.001%
35	4.613	1007	1018	1047	rBV	190033	466810	33.83%	4.074%
36	5.060	1140	1157	1182	rBV	278377	613360	44.45%	5.353%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051968.D
 Acq On : 20 Nov 2022 12:31
 Operator : JC/MD
 Sample : VU1120WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	5.292	1220	1229	1233	rBV3	1329	1775	0.13%	0.015%
38	5.343	1243	1245	1246	rBV	218	96	0.01%	0.001%
39	5.375	1251	1255	1257	rBV2	544	347	0.03%	0.003%
40	5.436	1269	1274	1275	rBV2	200	161	0.01%	0.001%
41	5.633	1331	1335	1340	rVB2	415	364	0.03%	0.003%
42	5.723	1341	1363	1396	rBV2	485305	1379791	100.00%	12.042%
43	5.916	1421	1423	1426	rBV	402	214	0.02%	0.002%
44	6.002	1447	1450	1453	rBV2	157	139	0.01%	0.001%
45	6.044	1460	1463	1467	rVB2	430	334	0.02%	0.003%
46	6.108	1477	1483	1485	rBV2	281	299	0.02%	0.003%
47	6.157	1495	1498	1503	rVB2	268	241	0.02%	0.002%
48	6.186	1504	1507	1511	rBV2	161	112	0.01%	0.001%
49	6.247	1511	1526	1554	rBV	522700	1008762	73.11%	8.804%
50	6.536	1606	1616	1629	rVB9	4426	9776	0.71%	0.085%
51	6.597	1629	1635	1638	rBV3	445	377	0.03%	0.003%
52	6.687	1649	1663	1685	rBV	356089	699171	50.67%	6.102%
53	6.870	1716	1720	1722	rBV	232	134	0.01%	0.001%
54	6.922	1734	1736	1739	rVB	194	79	0.01%	0.001%
55	6.967	1747	1750	1753	rVB2	216	134	0.01%	0.001%
56	7.047	1772	1775	1780	rVB	170	144	0.01%	0.001%
57	7.073	1780	1783	1785	rBV2	127	85	0.01%	0.001%
58	7.134	1800	1802	1806	rVB2	159	92	0.01%	0.001%
59	7.182	1806	1817	1835	rBV3	5939	11669	0.85%	0.102%
60	7.292	1850	1851	1855	rBV2	151	87	0.01%	0.001%
61	7.353	1869	1870	1873	rVB	243	90	0.01%	0.001%
62	7.475	1906	1908	1914	rVB	182	127	0.01%	0.001%
63	7.562	1923	1935	1959	rBV	145802	259200	18.79%	2.262%
64	7.694	1966	1976	1985	rBV4	4066	7164	0.52%	0.063%
65	7.764	1995	1998	2003	rVB3	285	205	0.01%	0.002%
66	7.796	2005	2008	2010	rBV3	497	364	0.03%	0.003%
67	7.838	2018	2021	2026	rBV2	224	208	0.02%	0.002%
68	7.896	2026	2039	2063	rBV	481178	838033	60.74%	7.314%
69	8.134	2110	2113	2115	rBV	211	128	0.01%	0.001%
70	8.176	2115	2126	2145	rBV	102928	176412	12.79%	1.540%
71	8.533	2232	2237	2238	rBV2	255	199	0.01%	0.002%
72	8.555	2238	2244	2248	rVB4	611	773	0.06%	0.007%
73	8.632	2255	2268	2300	rBV2	528362	1002971	72.69%	8.753%
74	8.976	2374	2375	2377	rBV	259	87	0.01%	0.001%
75	9.076	2403	2406	2407	rBV	262	129	0.01%	0.001%
76	9.128	2419	2422	2423	rBV	289	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051968.D
 Acq On : 20 Nov 2022 12:31
 Operator : JC/MD
 Sample : VU1120WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	9.147	2427	2428	2430	rBV2	185	69	0.01%	0.001%
78	9.163	2430	2433	2435	rBV	178	113	0.01%	0.001%
79	9.230	2450	2454	2457	rBV	314	274	0.02%	0.002%
80	9.292	2470	2473	2478	rBV2	417	328	0.02%	0.003%
81	9.414	2498	2511	2550	rBV	780262	1292245	93.66%	11.278%
82	9.671	2587	2591	2595	rBV2	663	740	0.05%	0.006%
83	10.378	2808	2811	2813	rBV2	282	203	0.01%	0.002%
84	10.755	2914	2928	2955	rBV	675039	1075821	77.97%	9.389%
85	10.980	2996	2998	3003	rBV2	344	221	0.02%	0.002%
86	11.086	3028	3031	3032	rBV	484	296	0.02%	0.003%
87	11.144	3045	3049	3050	rBV	267	186	0.01%	0.002%
88	11.266	3085	3087	3089	rBV2	189	122	0.01%	0.001%
89	11.337	3106	3109	3111	rBV	159	112	0.01%	0.001%
90	11.555	3174	3177	3180	rBV	390	276	0.02%	0.002%
91	11.584	3184	3186	3189	rVB2	478	253	0.02%	0.002%
92	11.809	3243	3256	3286	rBV	572198	930182	67.41%	8.118%
93	11.999	3312	3315	3318	rVB2	684	447	0.03%	0.004%
94	12.018	3318	3321	3324	rBV	466	354	0.03%	0.003%
95	12.192	3361	3375	3401	rBV	591590	969633	70.27%	8.462%
96	13.330	3727	3729	3732	rBV2	498	252	0.02%	0.002%
97	13.841	3882	3888	3896	rBV5	3481	5288	0.38%	0.046%
98	13.906	3905	3908	3910	rBV2	484	307	0.02%	0.003%
99	14.092	3959	3966	3981	rBV2	5999	10500	0.76%	0.092%
100	14.333	4035	4041	4054	rVB5	4308	7178	0.52%	0.063%




Sum of corrected areas: 11458159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051968.D
Acq On : 20 Nov 2022 12:31
Operator : JC/MD
Sample : VU1120WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

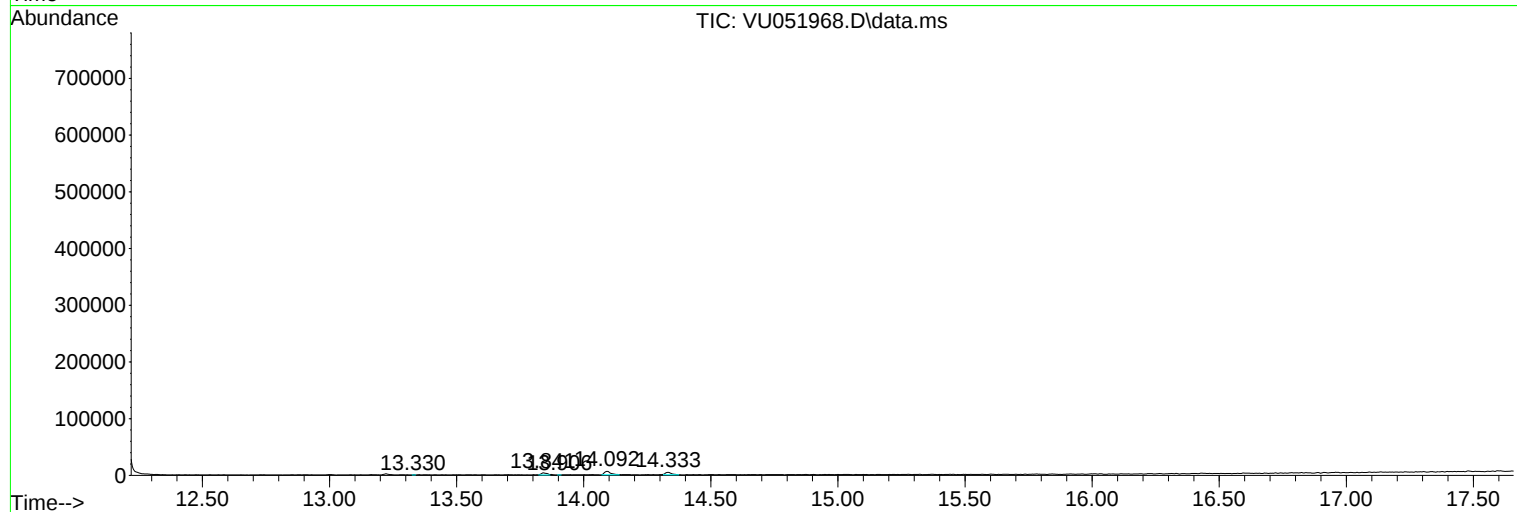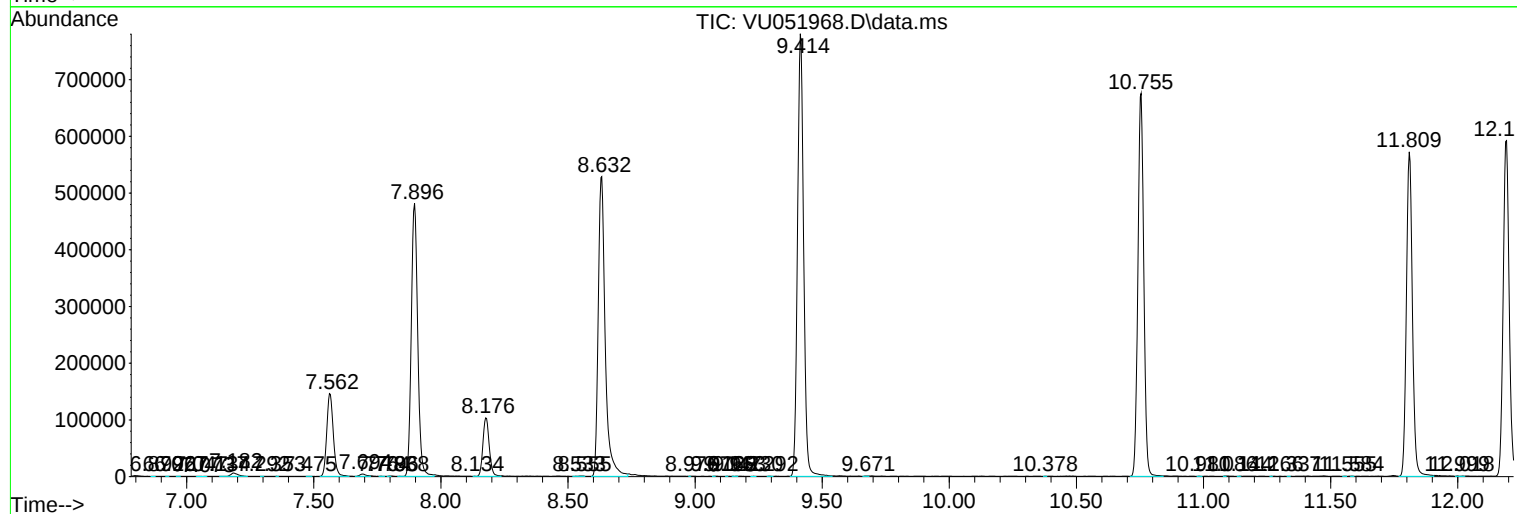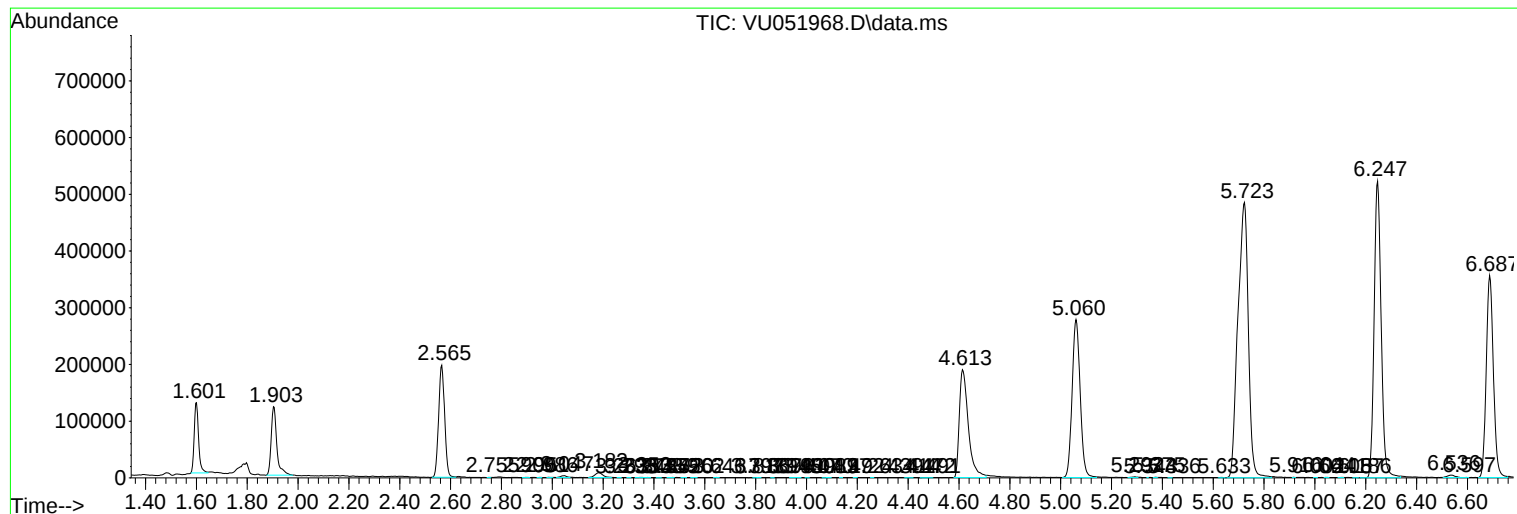

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051968.D
Acq On : 20 Nov 2022 12:31
Operator : JC/MD
Sample : VU1120WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051968.D
Acq On : 20 Nov 2022 12:31
Operator : JC/MD
Sample : VU1120WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc