

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051969.D
 Acq On : 20 Nov 2022 13:01
 Operator : JC/MD
 Sample : N5683-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	113808	134060	10.38%	1.230%
2	1.906	167	176	198	rVB	112470	167214	12.95%	1.534%
3	2.565	369	381	394	rBV	181638	296120	22.93%	2.717%
4	2.707	422	425	431	rVB2	447	341	0.03%	0.003%
5	2.787	445	450	460	rBV4	819	1222	0.09%	0.011%
6	3.002	513	517	519	rBV2	290	229	0.02%	0.002%
7	3.047	523	531	539	rVV6	1812	3003	0.23%	0.028%
8	3.170	564	569	570	rBV2	727	544	0.04%	0.005%
9	3.334	614	620	624	rBV3	278	274	0.02%	0.003%
10	3.520	672	678	681	rBV	344	369	0.03%	0.003%
11	3.986	818	823	828	rVB	233	261	0.02%	0.002%
12	4.012	828	831	836	rBV	251	236	0.02%	0.002%
13	4.125	864	866	873	rVB2	261	225	0.02%	0.002%
14	4.195	884	888	893	rVB2	279	280	0.02%	0.003%
15	4.616	1007	1019	1046	rBV	165409	406241	31.46%	3.727%
16	5.060	1141	1157	1186	rBV	263712	575837	44.59%	5.283%
17	5.285	1220	1227	1231	rBV5	1138	1423	0.11%	0.013%
18	5.372	1250	1254	1258	rBV3	638	669	0.05%	0.006%
19	5.723	1342	1363	1390	rBV2	451721	1288054	99.75%	11.817%
20	5.912	1419	1422	1427	rBV3	539	416	0.03%	0.004%
21	6.044	1460	1463	1467	rVB3	247	238	0.02%	0.002%
22	6.169	1498	1502	1508	rVB2	436	332	0.03%	0.003%
23	6.247	1511	1526	1555	rBV	524275	1006941	77.98%	9.238%
24	6.491	1598	1602	1605	rBV2	338	360	0.03%	0.003%
25	6.539	1607	1617	1625	rVV8	3268	6303	0.49%	0.058%
26	6.687	1646	1663	1686	rBV	336444	660463	51.15%	6.059%
27	7.115	1793	1796	1800	rVV2	348	264	0.02%	0.002%
28	7.186	1808	1818	1832	rVV4	5658	11114	0.86%	0.102%
29	7.240	1832	1835	1840	rVB3	213	233	0.02%	0.002%
30	7.565	1923	1936	1955	rVV	137092	239839	18.57%	2.200%
31	7.690	1969	1975	1985	rBV3	2886	4565	0.35%	0.042%
32	7.800	2004	2009	2012	rVB2	360	372	0.03%	0.003%
33	7.896	2020	2039	2059	rBV	448326	783622	60.69%	7.189%
34	8.105	2100	2104	2111	rBV4	412	438	0.03%	0.004%
35	8.179	2116	2127	2147	rVV	97004	165631	12.83%	1.520%
36	8.388	2189	2192	2196	rVB2	463	292	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051969.D
 Acq On : 20 Nov 2022 13:01
 Operator : JC/MD
 Sample : N5683-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	8.468	2211	2217	2229	rVB3	1956	3050	0.24%	0.028%
38	8.552	2238	2243	2244	rBV4	479	395	0.03%	0.004%
39	8.632	2253	2268	2305	rBV2	467460	905098	70.09%	8.304%
40	8.848	2334	2335	2338	rVB2	659	268	0.02%	0.002%
41	9.018	2384	2388	2391	rBV	567	403	0.03%	0.004%
42	9.166	2430	2434	2438	rVV3	380	310	0.02%	0.003%
43	9.292	2470	2473	2480	rVB	301	310	0.02%	0.003%
44	9.330	2480	2485	2488	rBV	411	416	0.03%	0.004%
45	9.414	2498	2511	2538	rBV	780478	1291285	100.00%	11.847%
46	9.568	2557	2559	2565	rVB3	805	744	0.06%	0.007%
47	9.693	2595	2598	2606	rVB4	512	640	0.05%	0.006%
48	9.774	2620	2623	2626	rBV2	502	272	0.02%	0.002%
49	9.883	2653	2657	2664	rVB3	425	502	0.04%	0.005%
50	9.922	2664	2669	2677	rBV2	276	485	0.04%	0.004%
51	10.076	2713	2717	2720	rVB	349	247	0.02%	0.002%
52	10.484	2838	2844	2846	rBV3	355	409	0.03%	0.004%
53	10.636	2888	2891	2896	rVB2	443	393	0.03%	0.004%
54	10.755	2915	2928	2946	rBV	612568	996246	77.15%	9.140%
55	10.951	2984	2989	2993	rBV	272	249	0.02%	0.002%
56	11.095	3032	3034	3037	rVB	405	235	0.02%	0.002%
57	11.134	3042	3046	3051	rBV2	217	231	0.02%	0.002%
58	11.250	3079	3082	3086	rVB2	393	282	0.02%	0.003%
59	11.414	3131	3133	3139	rVB2	567	501	0.04%	0.005%
60	11.754	3232	3239	3244	rBV4	938	993	0.08%	0.009%
61	11.809	3244	3256	3286	rBV	598460	952316	73.75%	8.737%
62	12.005	3313	3317	3319	rBV2	398	353	0.03%	0.003%
63	12.070	3332	3337	3338	rBV4	1380	1151	0.09%	0.011%
64	12.121	3349	3353	3355	rBV2	396	264	0.02%	0.002%
65	12.192	3360	3375	3397	rBV	568062	940383	72.83%	8.627%
66	12.369	3426	3430	3431	rBV2	482	348	0.03%	0.003%
67	12.414	3439	3444	3445	rBV2	564	413	0.03%	0.004%
68	12.533	3477	3481	3483	rBV3	490	326	0.03%	0.003%
69	12.680	3524	3527	3533	rVB3	523	586	0.05%	0.005%
70	12.934	3599	3606	3610	rBV4	631	736	0.06%	0.007%
71	12.970	3613	3617	3620	rVV2	568	419	0.03%	0.004%
72	13.047	3637	3641	3644	rVV3	592	555	0.04%	0.005%
73	13.082	3648	3652	3654	rBV2	470	344	0.03%	0.003%
74	13.192	3682	3686	3688	rBV3	413	349	0.03%	0.003%
75	13.288	3714	3716	3719	rVB2	561	314	0.02%	0.003%
76	13.330	3724	3729	3733	rBV3	578	622	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051969.D
 Acq On : 20 Nov 2022 13:01
 Operator : JC/MD
 Sample : N5683-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	13.417	3752	3756	3759	rVB3	474	332	0.03%	0.003%
78	13.452	3759	3767	3777	rBV6	2065	3154	0.24%	0.029%
79	13.629	3816	3822	3828	rBV4	1411	1768	0.14%	0.016%
80	13.690	3837	3841	3848	rVB	472	562	0.04%	0.005%
81	13.719	3848	3850	3853	rBV	343	248	0.02%	0.002%
82	13.848	3882	3890	3896	rVB5	2619	3514	0.27%	0.032%
83	14.021	3942	3944	3950	rVB	493	416	0.03%	0.004%
84	14.092	3958	3966	3974	rBV2	4673	6585	0.51%	0.060%
85	14.143	3979	3982	3985	rBV2	452	324	0.03%	0.003%
86	14.192	3991	3997	4004	rVB4	2433	3090	0.24%	0.028%
87	14.224	4004	4007	4010	rBV2	344	268	0.02%	0.002%
88	14.291	4024	4028	4032	rVB6	921	904	0.07%	0.008%
89	14.333	4037	4041	4049	rVB5	2278	3114	0.24%	0.029%
90	14.369	4049	4052	4057	rBV3	838	673	0.05%	0.006%
91	14.391	4057	4059	4065	rVB3	422	430	0.03%	0.004%
92	14.475	4082	4085	4088	rBV3	683	574	0.04%	0.005%
93	14.532	4097	4103	4106	rBV3	584	585	0.05%	0.005%
94	14.671	4143	4146	4148	rBV2	1271	879	0.07%	0.008%
95	14.806	4184	4188	4195	rVB3	1480	1451	0.11%	0.013%
96	15.143	4290	4293	4294	rBV2	434	279	0.02%	0.003%
97	15.201	4305	4311	4313	rBV4	2073	2258	0.17%	0.021%
98	15.413	4368	4377	4387	rBV4	3474	5891	0.46%	0.054%
99	15.459	4388	4391	4395	rVV3	1048	696	0.05%	0.006%
100	15.632	4441	4445	4448	rBV3	860	640	0.05%	0.006%




Sum of corrected areas: 10900103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051969.D
Acq On : 20 Nov 2022 13:01
Operator : JC/MD
Sample : N5683-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

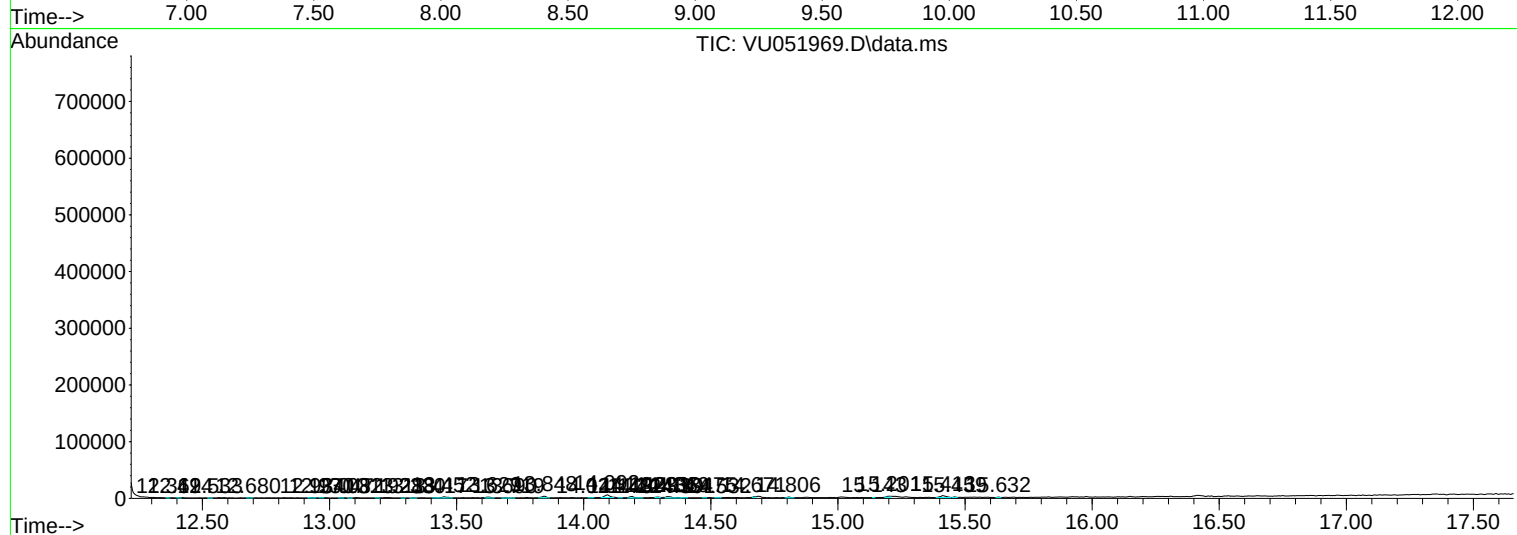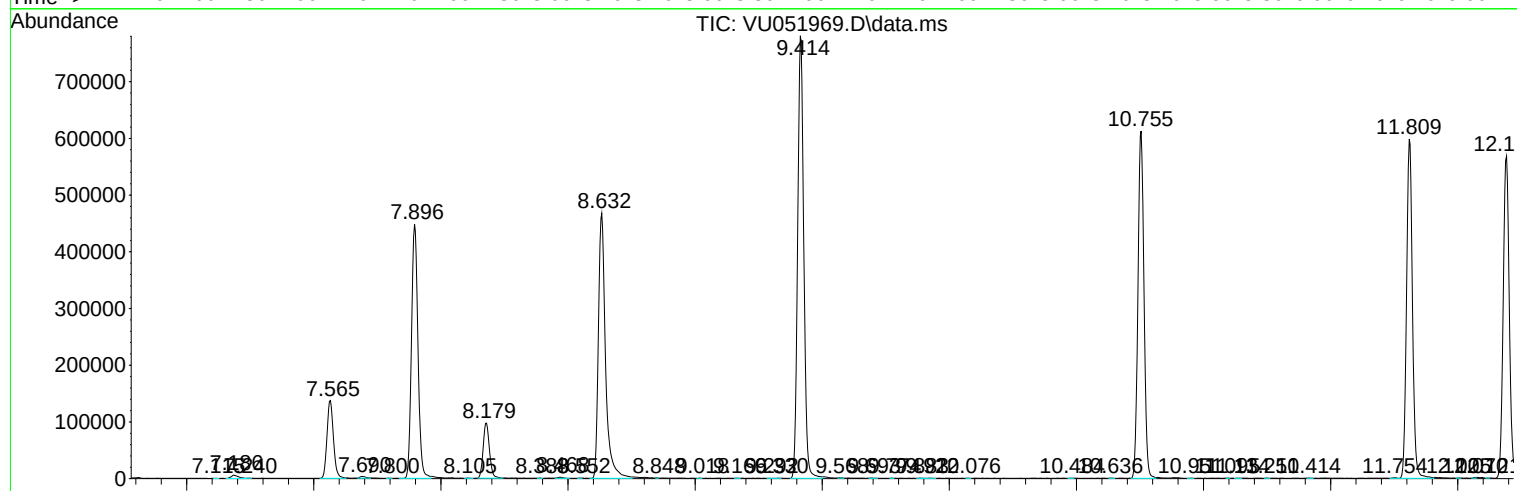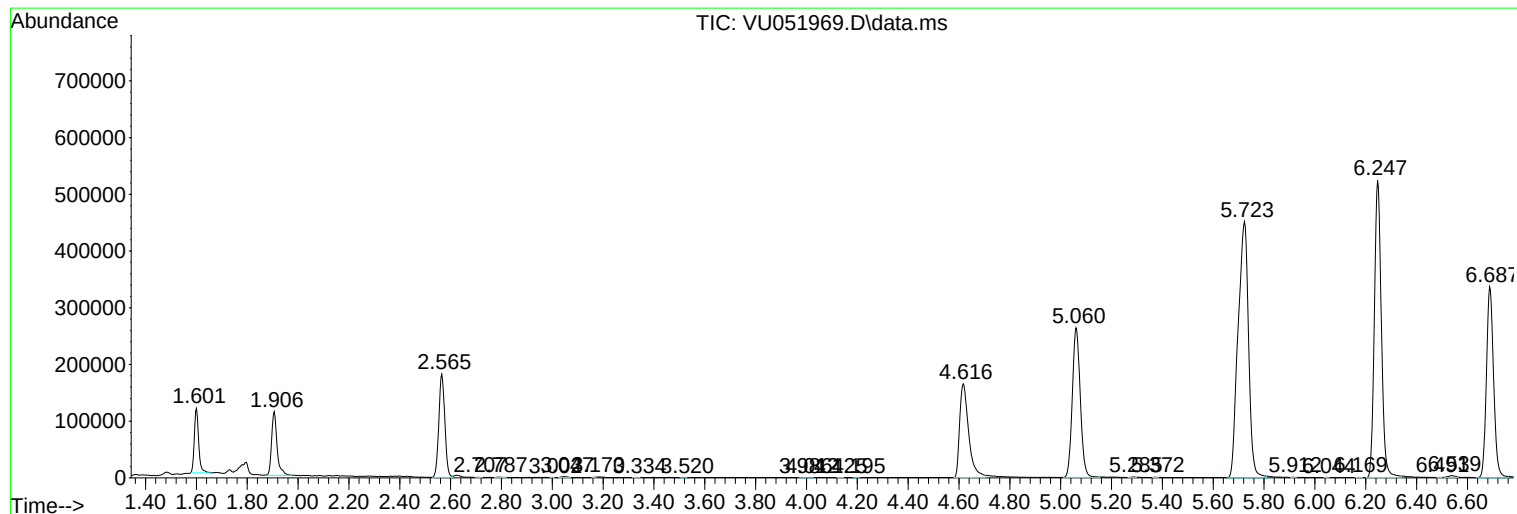

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051969.D
Acq On : 20 Nov 2022 13:01
Operator : JC/MD
Sample : N5683-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051969.D
Acq On : 20 Nov 2022 13:01
Operator : JC/MD
Sample : N5683-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc