

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051971.D
 Acq On : 20 Nov 2022 13:54
 Operator : JC/MD
 Sample : N5683-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.382	8	13	27	rVB	14561	19311	1.53%	0.182%
2	1.600	74	81	96	rBV	112961	131707	10.44%	1.243%
3	1.684	102	107	120	rVB2	17531	22285	1.77%	0.210%
4	1.906	168	176	200	rVB	110769	166228	13.17%	1.569%
5	2.565	366	381	393	rBV	179066	292274	23.16%	2.759%
6	2.623	394	399	415	rVB3	8397	15597	1.24%	0.147%
7	3.047	522	531	539	rVB5	1110	2129	0.17%	0.020%
8	3.176	564	571	574	rBV2	661	729	0.06%	0.007%
9	3.362	625	629	634	rBV	213	226	0.02%	0.002%
10	3.623	707	710	717	rVB	338	412	0.03%	0.004%
11	3.662	717	722	726	rBV2	450	461	0.04%	0.004%
12	3.713	736	738	745	rVB2	269	249	0.02%	0.002%
13	3.948	806	811	815	rBV2	290	304	0.02%	0.003%
14	3.999	824	827	835	rVB2	239	242	0.02%	0.002%
15	4.067	843	848	855	rVB2	315	370	0.03%	0.003%
16	4.234	897	900	907	rVB	283	285	0.02%	0.003%
17	4.475	971	975	981	rVB2	307	337	0.03%	0.003%
18	4.616	1006	1019	1047	rBV	171837	418723	33.18%	3.953%
19	5.060	1140	1157	1182	rBV	259876	570077	45.17%	5.382%
20	5.211	1202	1204	1208	rBV3	421	298	0.02%	0.003%
21	5.288	1218	1228	1231	rBV2	1049	1582	0.13%	0.015%
22	5.366	1249	1252	1253	rBV2	421	256	0.02%	0.002%
23	5.401	1257	1263	1264	rBV4	427	363	0.03%	0.003%
24	5.517	1295	1299	1304	rVB3	410	396	0.03%	0.004%
25	5.549	1304	1309	1312	rBV2	272	232	0.02%	0.002%
26	5.723	1341	1363	1383	rBV2	440487	1261987	100.00%	11.914%
27	5.986	1440	1445	1448	rBV2	393	330	0.03%	0.003%
28	6.166	1495	1501	1509	rBV2	335	418	0.03%	0.004%
29	6.247	1512	1526	1552	rBV	500392	965516	76.51%	9.115%
30	6.536	1608	1616	1629	rVB6	3123	5339	0.42%	0.050%
31	6.584	1629	1631	1637	rVB3	381	301	0.02%	0.003%
32	6.629	1640	1645	1648	rBV3	380	279	0.02%	0.003%
33	6.687	1648	1663	1693	rBV	328889	647995	51.35%	6.117%
34	6.903	1727	1730	1735	rBV	344	258	0.02%	0.002%
35	7.086	1784	1787	1789	rVB2	429	229	0.02%	0.002%
36	7.185	1809	1818	1830	rBV3	5161	9861	0.78%	0.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051971.D
 Acq On : 20 Nov 2022 13:54
 Operator : JC/MD
 Sample : N5683-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	7.562	1920	1935	1952	rBV	134773	239432	18.97%	2.260%
38	7.690	1968	1975	1987	rBV4	3879	6481	0.51%	0.061%
39	7.777	1998	2002	2004	rBV2	407	234	0.02%	0.002%
40	7.796	2004	2008	2009	rBV	605	321	0.03%	0.003%
41	7.806	2009	2011	2016	rVB2	664	559	0.04%	0.005%
42	7.848	2020	2024	2026	rBV	938	821	0.07%	0.008%
43	7.896	2026	2039	2062	rBV	442767	765262	60.64%	7.225%
44	8.128	2106	2111	2115	rVB3	587	641	0.05%	0.006%
45	8.176	2115	2126	2149	rBV	99933	166244	13.17%	1.569%
46	8.462	2209	2215	2220	rBV2	982	1190	0.09%	0.011%
47	8.552	2240	2243	2248	rVB5	536	506	0.04%	0.005%
48	8.629	2256	2267	2304	rBV2	477356	925019	73.30%	8.733%
49	8.845	2332	2334	2335	rBV2	469	252	0.02%	0.002%
50	8.877	2339	2344	2345	rBV2	497	293	0.02%	0.003%
51	8.893	2347	2349	2352	rVB2	497	256	0.02%	0.002%
52	8.928	2356	2360	2362	rBV	317	240	0.02%	0.002%
53	9.005	2381	2384	2388	rVV	346	260	0.02%	0.002%
54	9.041	2392	2395	2398	rVB3	410	221	0.02%	0.002%
55	9.137	2422	2425	2431	rBV2	218	250	0.02%	0.002%
56	9.214	2446	2449	2457	rVB	261	296	0.02%	0.003%
57	9.414	2498	2511	2545	rBV	733253	1221674	96.81%	11.533%
58	9.584	2562	2564	2568	rVB	802	479	0.04%	0.005%
59	9.748	2610	2615	2617	rBV2	480	419	0.03%	0.004%
60	9.989	2686	2690	2697	rVB2	397	521	0.04%	0.005%
61	10.095	2718	2723	2725	rBV2	254	263	0.02%	0.002%
62	10.121	2729	2731	2736	rVB3	562	388	0.03%	0.004%
63	10.340	2796	2799	2804	rBV2	330	282	0.02%	0.003%
64	10.372	2805	2809	2815	rBV2	264	270	0.02%	0.003%
65	10.613	2881	2884	2888	rVB2	409	248	0.02%	0.002%
66	10.751	2914	2927	2955	rBV	595493	968368	76.73%	9.142%
67	10.883	2964	2968	2972	rBV5	806	910	0.07%	0.009%
68	11.015	3006	3009	3013	rBV2	468	312	0.02%	0.003%
69	11.089	3029	3032	3037	rVV2	325	289	0.02%	0.003%
70	11.111	3037	3039	3046	rVV2	308	292	0.02%	0.003%
71	11.346	3107	3112	3119	rVB2	308	450	0.04%	0.004%
72	11.635	3198	3202	3209	rBV3	394	533	0.04%	0.005%
73	11.687	3215	3218	3222	rVB2	381	258	0.02%	0.002%
74	11.748	3233	3237	3242	rVB3	606	660	0.05%	0.006%
75	11.809	3243	3256	3273	rBV	539861	862397	68.34%	8.142%
76	12.070	3328	3337	3352	rBV6	1534	3583	0.28%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051971.D
 Acq On : 20 Nov 2022 13:54
 Operator : JC/MD
 Sample : N5683-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3398	rBV	519882	870902	69.01%	8.222%
78	12.352	3422	3425	3428	rBV	413	247	0.02%	0.002%
79	12.668	3519	3523	3530	rVB5	2814	3022	0.24%	0.029%
80	12.758	3547	3551	3553	rBV	358	282	0.02%	0.003%
81	12.828	3570	3573	3580	rVB2	399	464	0.04%	0.004%
82	12.860	3580	3583	3585	rBV2	445	302	0.02%	0.003%
83	13.018	3629	3632	3635	rVV4	304	228	0.02%	0.002%
84	13.079	3648	3651	3654	rVB2	493	343	0.03%	0.003%
85	13.179	3679	3682	3684	rBV	393	299	0.02%	0.003%
86	13.224	3689	3696	3700	rBV4	577	839	0.07%	0.008%
87	13.275	3709	3712	3717	rBV	321	318	0.03%	0.003%
88	13.336	3726	3731	3733	rBV2	389	326	0.03%	0.003%
89	13.532	3789	3792	3795	rVV2	505	453	0.04%	0.004%
90	13.552	3795	3798	3800	rVB	632	310	0.02%	0.003%
91	13.661	3826	3832	3834	rBV3	514	440	0.03%	0.004%
92	13.803	3873	3876	3881	rVV2	441	418	0.03%	0.004%
93	13.909	3903	3909	3912	rBV2	467	540	0.04%	0.005%
94	14.098	3961	3968	3971	rBV3	1059	1210	0.10%	0.011%
95	14.333	4036	4041	4045	rBV4	727	774	0.06%	0.007%
96	14.381	4053	4056	4057	rBV	416	256	0.02%	0.002%
97	14.780	4177	4180	4186	rBV2	391	371	0.03%	0.004%
98	14.928	4224	4226	4230	rVB3	522	273	0.02%	0.003%
99	15.098	4276	4279	4283	rBV2	480	542	0.04%	0.005%
100	15.854	4512	4514	4517	rBV2	735	438	0.03%	0.004%




Sum of corrected areas: 10592557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051971.D
Acq On : 20 Nov 2022 13:54
Operator : JC/MD
Sample : N5683-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

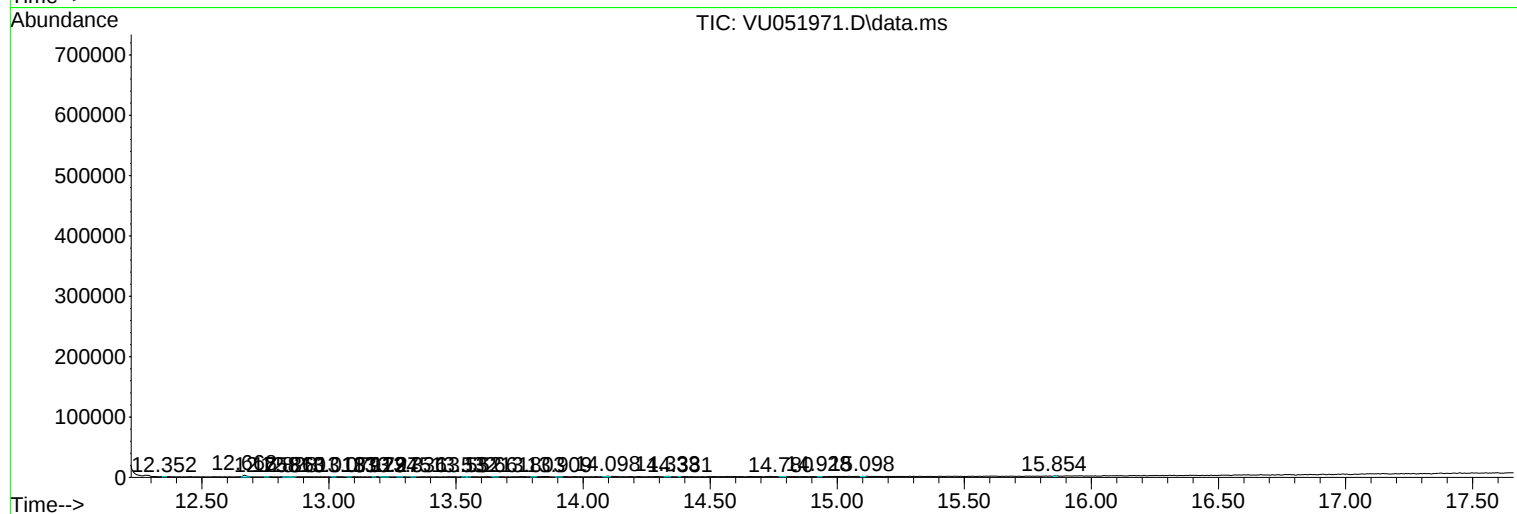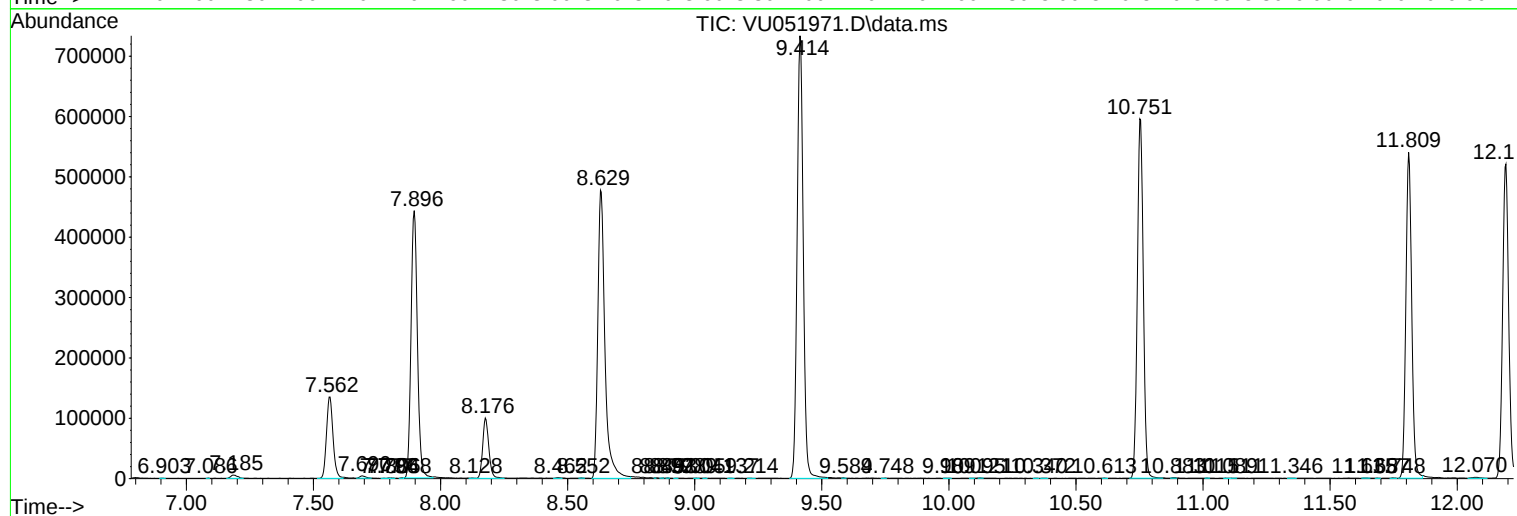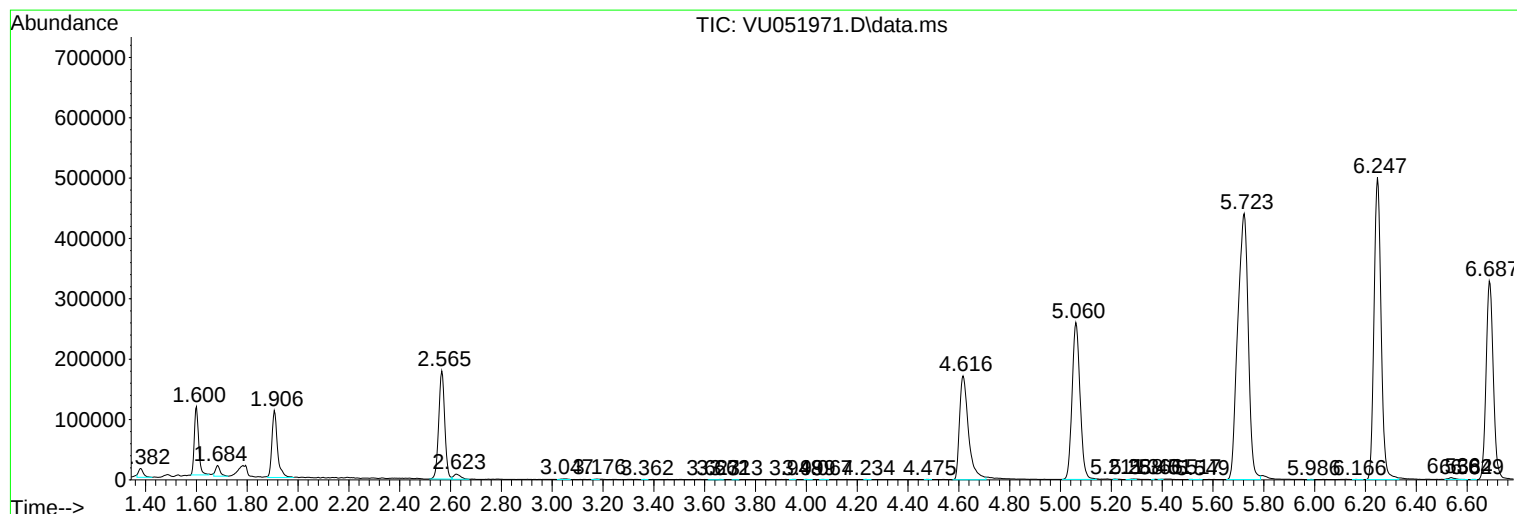

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051971.D
Acq On : 20 Nov 2022 13:54
Operator : JC/MD
Sample : N5683-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051971.D
Acq On : 20 Nov 2022 13:54
Operator : JC/MD
Sample : N5683-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc