

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051974.D
 Acq On : 20 Nov 2022 15:12
 Operator : JC/MD
 Sample : N5683-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	109829	127272	10.32%	1.226%
2	1.906	168	176	204	rVB	109260	166612	13.52%	1.605%
3	2.565	370	381	394	rBV	172659	280652	22.77%	2.703%
4	3.044	525	530	539	rVB2	1114	1627	0.13%	0.016%
5	3.124	553	555	558	rBV2	228	104	0.01%	0.001%
6	3.150	559	563	565	rBV	448	290	0.02%	0.003%
7	3.179	565	572	573	rBV2	820	939	0.08%	0.009%
8	3.253	588	595	596	rBV2	278	260	0.02%	0.003%
9	3.282	602	604	610	rVB	201	133	0.01%	0.001%
10	3.308	610	612	614	rVB	157	71	0.01%	0.001%
11	3.324	614	617	618	rBV2	269	148	0.01%	0.001%
12	3.359	627	628	631	rBV	260	125	0.01%	0.001%
13	3.391	635	638	639	rBV	294	162	0.01%	0.002%
14	3.530	678	681	683	rBV	255	176	0.01%	0.002%
15	3.587	689	699	709	rBV5	1869	3894	0.32%	0.038%
16	3.710	734	737	739	rBV	213	160	0.01%	0.002%
17	3.816	767	770	771	rBV	97	44	0.00%	0.000%
18	3.874	785	788	790	rBV	196	116	0.01%	0.001%
19	4.009	828	830	836	rBV2	103	116	0.01%	0.001%
20	4.031	836	837	838	rVV2	139	35	0.00%	0.000%
21	4.047	838	842	845	rVB	252	174	0.01%	0.002%
22	4.108	859	861	868	rBV2	336	395	0.03%	0.004%
23	4.166	877	879	881	rBV2	110	50	0.00%	0.000%
24	4.237	896	901	907	rBV2	154	170	0.01%	0.002%
25	4.298	917	920	925	rVB	378	289	0.02%	0.003%
26	4.321	925	927	929	rBV	118	68	0.01%	0.001%
27	4.372	939	943	946	rBV2	282	235	0.02%	0.002%
28	4.407	951	954	956	rBV	212	149	0.01%	0.001%
29	4.472	968	974	976	rBV2	188	229	0.02%	0.002%
30	4.485	976	978	979	rBV	163	54	0.00%	0.001%
31	4.523	988	990	995	rBV	161	119	0.01%	0.001%
32	4.616	1007	1019	1053	rBV	165373	410173	33.27%	3.951%
33	5.060	1141	1157	1183	rBV2	253057	556007	45.10%	5.356%
34	5.263	1217	1220	1221	rBV2	270	171	0.01%	0.002%
35	5.356	1244	1249	1250	rBV2	198	182	0.01%	0.002%
36	5.366	1250	1252	1254	rBV	237	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051974.D
 Acq On : 20 Nov 2022 15:12
 Operator : JC/MD
 Sample : N5683-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	5.558	1308	1312	1315	rBV2	249	214	0.02%	0.002%
38	5.722	1342	1363	1377	rBV2	434501	1232726	100.00%	11.874%
39	6.009	1449	1452	1458	rBV2	292	327	0.03%	0.003%
40	6.054	1464	1466	1469	rBV	116	61	0.00%	0.001%
41	6.086	1474	1476	1478	rBV	228	105	0.01%	0.001%
42	6.105	1478	1482	1484	rBV2	294	226	0.02%	0.002%
43	6.124	1487	1488	1490	rBV	256	101	0.01%	0.001%
44	6.160	1495	1499	1501	rBV2	380	306	0.02%	0.003%
45	6.192	1507	1509	1512	rBV2	247	96	0.01%	0.001%
46	6.247	1512	1526	1551	rBV	507587	970258	78.71%	9.346%
47	6.452	1588	1590	1594	rVB2	345	176	0.01%	0.002%
48	6.478	1595	1598	1601	rVB3	413	256	0.02%	0.002%
49	6.536	1607	1616	1618	rBV5	2326	3093	0.25%	0.030%
50	6.581	1628	1630	1633	rVB2	408	193	0.02%	0.002%
51	6.687	1648	1663	1694	rBV	323519	637194	51.69%	6.138%
52	6.899	1726	1729	1730	rBV	134	72	0.01%	0.001%
53	6.960	1746	1748	1752	rVB2	260	131	0.01%	0.001%
54	6.989	1752	1757	1762	rBV2	329	450	0.04%	0.004%
55	7.095	1788	1790	1796	rVB2	254	211	0.02%	0.002%
56	7.185	1808	1818	1835	rVB3	5773	11297	0.92%	0.109%
57	7.250	1835	1838	1840	rBV	122	82	0.01%	0.001%
58	7.298	1851	1853	1855	rBV2	189	91	0.01%	0.001%
59	7.346	1865	1868	1871	rBV	228	181	0.01%	0.002%
60	7.465	1904	1905	1907	rBV	112	38	0.00%	0.000%
61	7.562	1923	1935	1953	rBV	131128	233262	18.92%	2.247%
62	7.690	1968	1975	1985	rBV5	3265	6036	0.49%	0.058%
63	7.748	1990	1993	1996	rBV2	309	255	0.02%	0.002%
64	7.845	2022	2023	2026	rBV2	199	78	0.01%	0.001%
65	7.896	2026	2039	2063	rBV	435822	752690	61.06%	7.250%
66	8.105	2099	2104	2107	rBV2	360	393	0.03%	0.004%
67	8.176	2114	2126	2148	rBV2	92229	161404	13.09%	1.555%
68	8.629	2253	2267	2307	rBV2	454416	899797	72.99%	8.667%
69	8.877	2342	2344	2348	rVB2	435	197	0.02%	0.002%
70	8.938	2360	2363	2365	rBV2	364	267	0.02%	0.003%
71	9.108	2413	2416	2418	rBV2	326	194	0.02%	0.002%
72	9.134	2422	2424	2425	rBV	298	95	0.01%	0.001%
73	9.214	2446	2449	2452	rBV	289	190	0.02%	0.002%
74	9.304	2475	2477	2480	rBV2	267	126	0.01%	0.001%
75	9.414	2498	2511	2529	rBV	741468	1224794	99.36%	11.797%
76	10.433	2826	2828	2831	rBV	248	169	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051974.D
 Acq On : 20 Nov 2022 15:12
 Operator : JC/MD
 Sample : N5683-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M

Title : VOC Analysis

77	10.491	2843	2846	2849	rBV3	462	263	0.02%	0.003%
78	10.754	2915	2928	2946	rBV	583889	949920	77.06%	9.150%
79	10.922	2978	2980	2983	rBV	326	210	0.02%	0.002%
80	11.066	3022	3025	3028	rBV2	413	269	0.02%	0.003%
81	11.809	3243	3256	3286	rBV	556993	887297	71.98%	8.547%
82	12.188	3362	3374	3391	rBV	518894	854402	69.31%	8.230%
83	12.471	3459	3462	3463	rBV2	262	162	0.01%	0.002%


Sum of corrected areas: 10381876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051974.D
Acq On : 20 Nov 2022 15:12
Operator : JC/MD
Sample : N5683-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

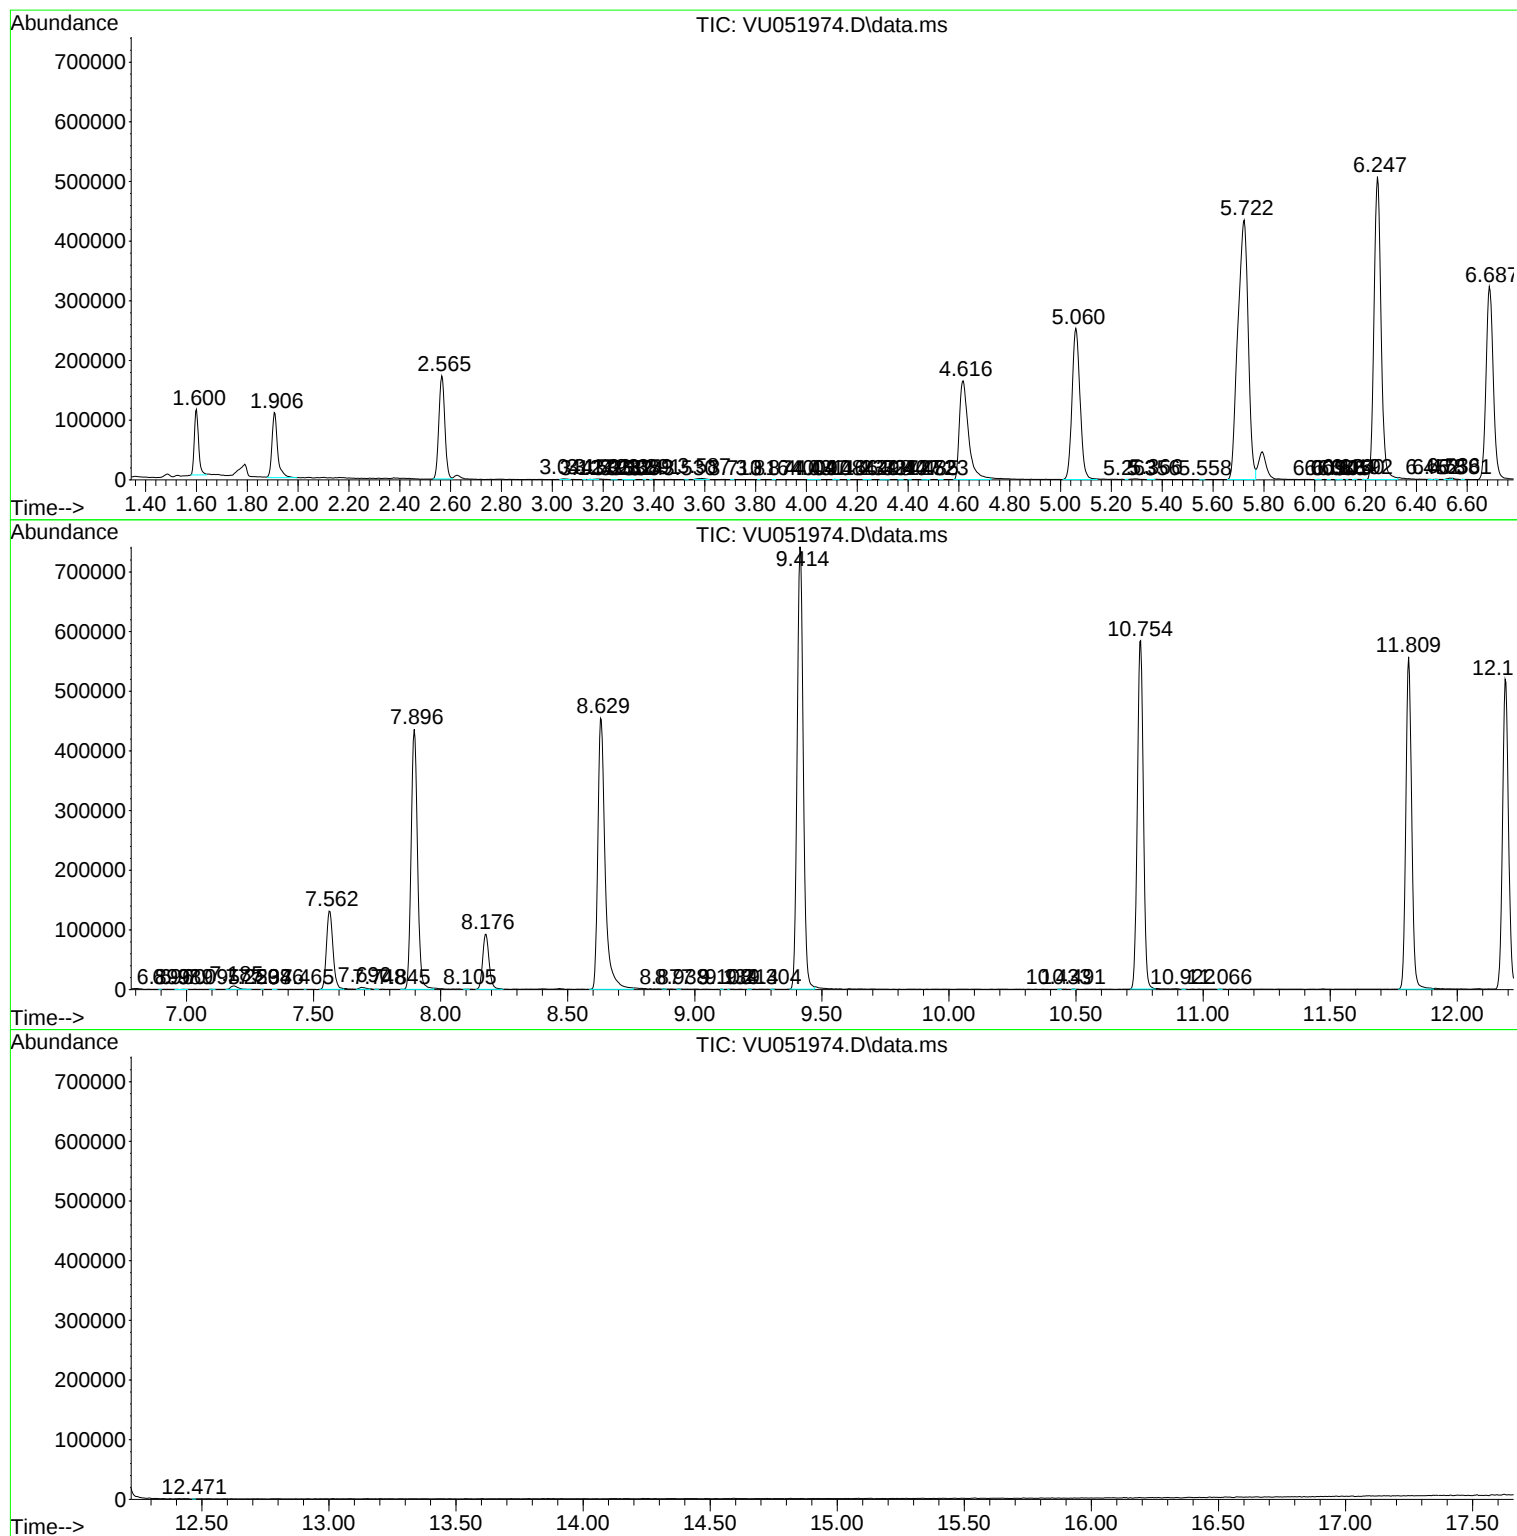

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051974.D
Acq On : 20 Nov 2022 15:12
Operator : JC/MD
Sample : N5683-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051974.D
Acq On : 20 Nov 2022 15:12
Operator : JC/MD
Sample : N5683-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------