

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051979.D
 Acq On : 20 Nov 2022 17:22
 Operator : JC/MD
 Sample : N5710-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COKY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	109399	129606	9.89%	1.053%
2	1.906	169	176	196	rVB	105867	160190	12.22%	1.302%
3	2.565	369	381	395	rBV2	181549	318295	24.29%	2.586%
4	3.002	513	517	518	rBV2	354	254	0.02%	0.002%
5	3.041	523	529	532	rBV3	852	1054	0.08%	0.009%
6	3.420	644	647	650	rBV	214	126	0.01%	0.001%
7	3.507	667	674	678	rBV2	340	441	0.03%	0.004%
8	3.552	686	688	690	rVB2	140	35	0.00%	0.000%
9	3.732	742	744	746	rBV	138	68	0.01%	0.001%
10	3.748	746	749	751	rBV	249	154	0.01%	0.001%
11	3.793	759	763	765	rBV	204	117	0.01%	0.001%
12	3.871	771	787	803	rVB2	5637	12445	0.95%	0.101%
13	3.935	804	807	808	rBV	131	76	0.01%	0.001%
14	3.993	822	825	826	rBV	191	103	0.01%	0.001%
15	4.041	838	840	842	rBV	200	80	0.01%	0.001%
16	4.054	842	844	847	rBV2	224	137	0.01%	0.001%
17	4.105	859	860	861	rBV2	107	31	0.00%	0.000%
18	4.250	901	905	910	rVB3	449	385	0.03%	0.003%
19	4.276	910	913	915	rBV2	165	111	0.01%	0.001%
20	4.317	923	926	930	rVB2	214	163	0.01%	0.001%
21	4.337	930	932	936	rVB	286	173	0.01%	0.001%
22	4.379	939	945	948	rVB2	236	267	0.02%	0.002%
23	4.404	948	953	957	rBV2	294	320	0.02%	0.003%
24	4.424	957	959	962	rVB	173	89	0.01%	0.001%
25	4.459	966	970	974	rBV	315	239	0.02%	0.002%
26	4.616	996	1019	1025	rBV	169547	363203	27.71%	2.951%
27	5.060	1142	1157	1177	rBV	255971	561632	42.85%	4.564%
28	5.314	1224	1236	1252	rVB5	7369	16792	1.28%	0.136%
29	5.469	1282	1284	1291	rVB2	422	310	0.02%	0.003%
30	5.501	1291	1294	1298	rBV2	166	97	0.01%	0.001%
31	5.523	1298	1301	1304	rVB2	269	170	0.01%	0.001%
32	5.539	1304	1306	1308	rBV	216	75	0.01%	0.001%
33	5.559	1308	1312	1316	rBV2	150	136	0.01%	0.001%
34	5.626	1330	1333	1335	rBV	142	95	0.01%	0.001%
35	5.723	1341	1363	1402	rBV2	438971	1262445	96.32%	10.258%
36	5.986	1442	1445	1446	rBV	317	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051979.D
 Acq On : 20 Nov 2022 17:22
 Operator : JC/MD
 Sample : N5710-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	6.115	1481	1485	1489	rBV3	555	594	0.05%	0.005%
38	6.247	1509	1526	1557	rBV	514136	982569	74.97%	7.984%
39	6.465	1590	1594	1599	rBV5	499	594	0.05%	0.005%
40	6.539	1604	1617	1639	rBV	226083	428948	32.73%	3.485%
41	6.687	1649	1663	1693	rBV	328749	638618	48.73%	5.189%
42	6.858	1713	1716	1717	rBV	245	119	0.01%	0.001%
43	6.899	1727	1729	1736	rVB2	430	342	0.03%	0.003%
44	6.928	1736	1738	1740	rVB	57	22	0.00%	0.000%
45	6.944	1740	1743	1744	rBV	281	170	0.01%	0.001%
46	7.099	1783	1791	1794	rBV4	983	1002	0.08%	0.008%
47	7.186	1809	1818	1832	rBV4	5537	10750	0.82%	0.087%
48	7.276	1841	1846	1851	rVB3	266	267	0.02%	0.002%
49	7.301	1851	1854	1857	rBV2	167	109	0.01%	0.001%
50	7.321	1857	1860	1862	rBV2	182	113	0.01%	0.001%
51	7.337	1862	1865	1868	rBV	272	155	0.01%	0.001%
52	7.385	1876	1880	1885	rBV2	371	336	0.03%	0.003%
53	7.414	1885	1889	1892	rBV2	214	223	0.02%	0.002%
54	7.446	1897	1899	1900	rBV	113	54	0.00%	0.000%
55	7.517	1918	1921	1923	rVB	270	152	0.01%	0.001%
56	7.562	1923	1935	1952	rBV	133123	238698	18.21%	1.940%
57	7.690	1968	1975	1993	rVB3	3950	7688	0.59%	0.062%
58	7.764	1996	1998	2001	rBV3	224	135	0.01%	0.001%
59	7.841	2019	2022	2024	rBV	202	152	0.01%	0.001%
60	7.896	2026	2039	2069	rVV	444934	772263	58.92%	6.275%
61	8.128	2108	2111	2114	rBV2	374	312	0.02%	0.003%
62	8.179	2115	2127	2150	rVV	95388	163322	12.46%	1.327%
63	8.288	2158	2161	2163	rBV2	664	286	0.02%	0.002%
64	8.443	2205	2209	2213	rBV2	494	484	0.04%	0.004%
65	8.468	2215	2217	2226	rVB4	1216	1563	0.12%	0.013%
66	8.549	2229	2242	2257	rBV	774784	1310653	100.00%	10.650%
67	8.629	2257	2267	2311	rVB2	471871	908247	69.30%	7.380%
68	9.089	2408	2410	2411	rBV	198	83	0.01%	0.001%
69	9.169	2432	2435	2440	rBV3	267	285	0.02%	0.002%
70	9.285	2465	2471	2475	rBV2	368	338	0.03%	0.003%
71	9.308	2475	2478	2482	rBV3	365	427	0.03%	0.003%
72	9.353	2489	2492	2495	rBV2	295	177	0.01%	0.001%
73	9.414	2498	2511	2536	rBV	756333	1243261	94.86%	10.102%
74	9.648	2581	2584	2589	rBV2	315	316	0.02%	0.003%
75	9.703	2599	2601	2607	rBV2	318	254	0.02%	0.002%
76	9.854	2644	2648	2650	rBV	401	305	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
 Data File : VU051979.D
 Acq On : 20 Nov 2022 17:22
 Operator : JC/MD
 Sample : N5710-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	9.957	2677	2680	2681	rBV	158	92	0.01%	0.001%
78	10.092	2720	2722	2726	rBV	297	214	0.02%	0.002%
79	10.253	2768	2772	2774	rBV2	461	274	0.02%	0.002%
80	10.349	2800	2802	2805	rVB	154	47	0.00%	0.000%
81	10.414	2819	2822	2827	rVB2	229	212	0.02%	0.002%
82	10.449	2830	2833	2834	rBV	280	126	0.01%	0.001%
83	10.500	2847	2849	2852	rBV2	249	160	0.01%	0.001%
84	10.539	2859	2861	2863	rBV	245	132	0.01%	0.001%
85	10.674	2901	2903	2910	rVB	385	300	0.02%	0.002%
86	10.700	2910	2911	2912	rBV	141	38	0.00%	0.000%
87	10.751	2915	2927	2954	rBV	593044	955794	72.93%	7.766%
88	11.240	3075	3079	3083	rBV2	618	486	0.04%	0.004%
89	11.295	3094	3096	3097	rBV2	166	54	0.00%	0.000%
90	11.340	3106	3110	3113	rBV3	304	227	0.02%	0.002%
91	11.594	3185	3189	3191	rBV	359	295	0.02%	0.002%
92	11.809	3243	3256	3277	rBV	555147	894691	68.26%	7.270%
93	12.060	3326	3334	3348	rBV3	11903	21815	1.66%	0.177%
94	12.189	3362	3374	3406	rBV	531989	886750	67.66%	7.205%
95	12.623	3506	3509	3512	rBV3	296	246	0.02%	0.002%
96	13.886	3899	3902	3907	rBV2	535	580	0.04%	0.005%




Sum of corrected areas: 12307005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051979.D
Acq On : 20 Nov 2022 17:22
Operator : JC/MD
Sample : N5710-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

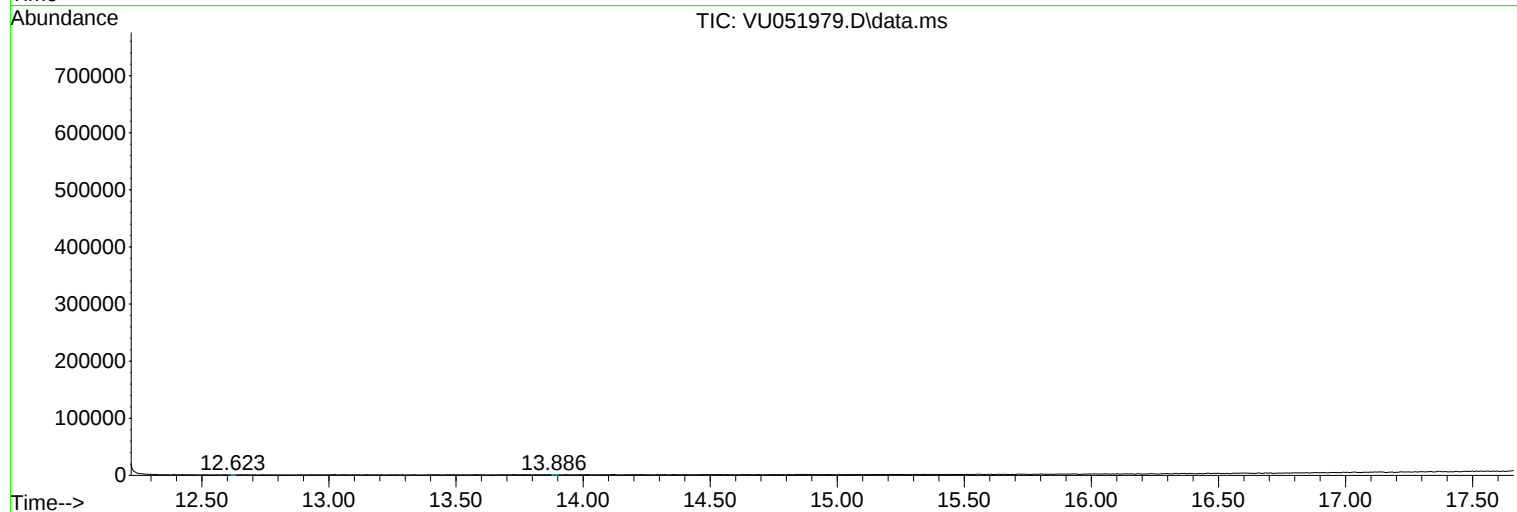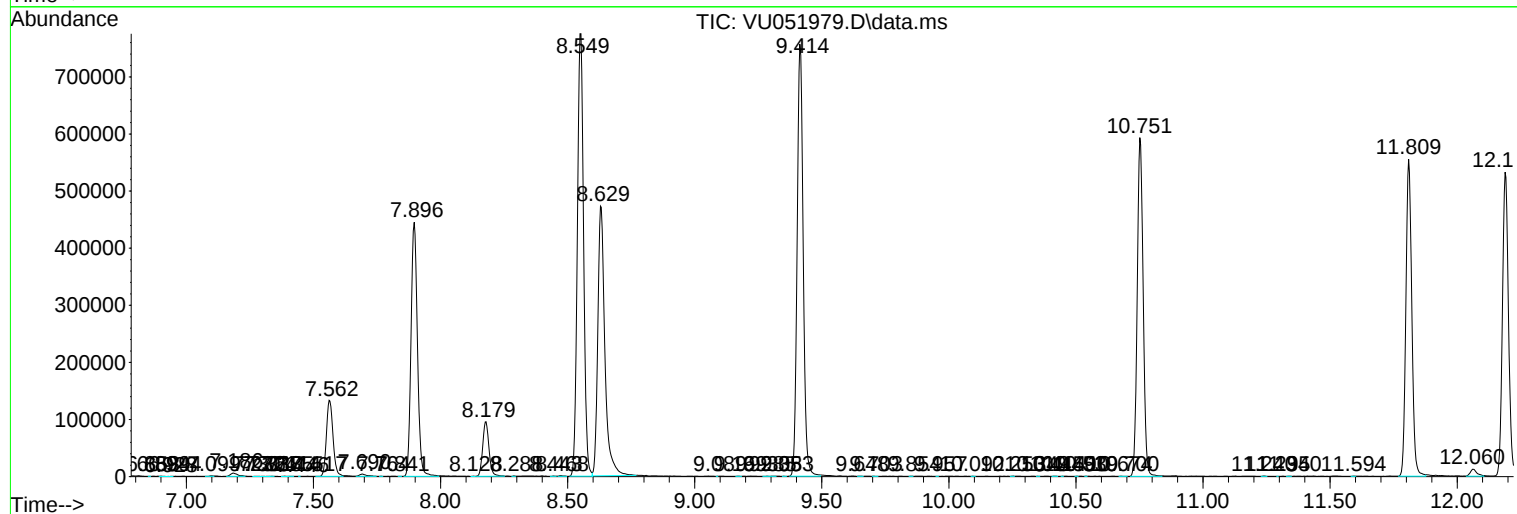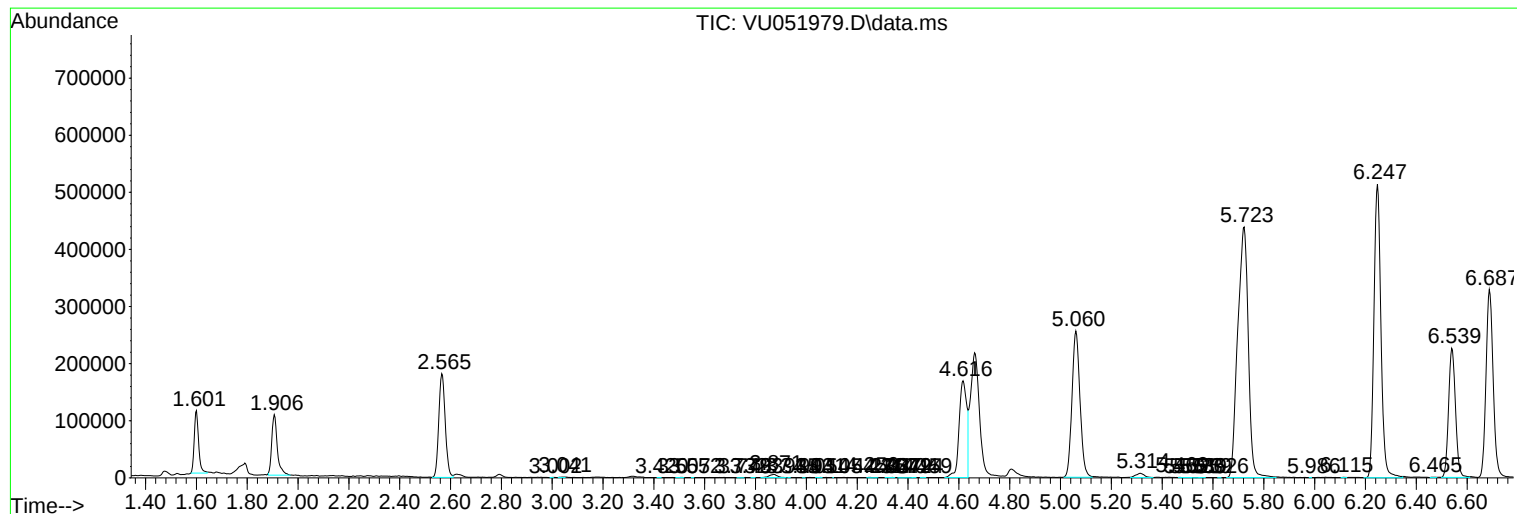

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051979.D
Acq On : 20 Nov 2022 17:22
Operator : JC/MD
Sample : N5710-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051979.D
Acq On : 20 Nov 2022 17:22
Operator : JC/MD
Sample : N5710-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc