
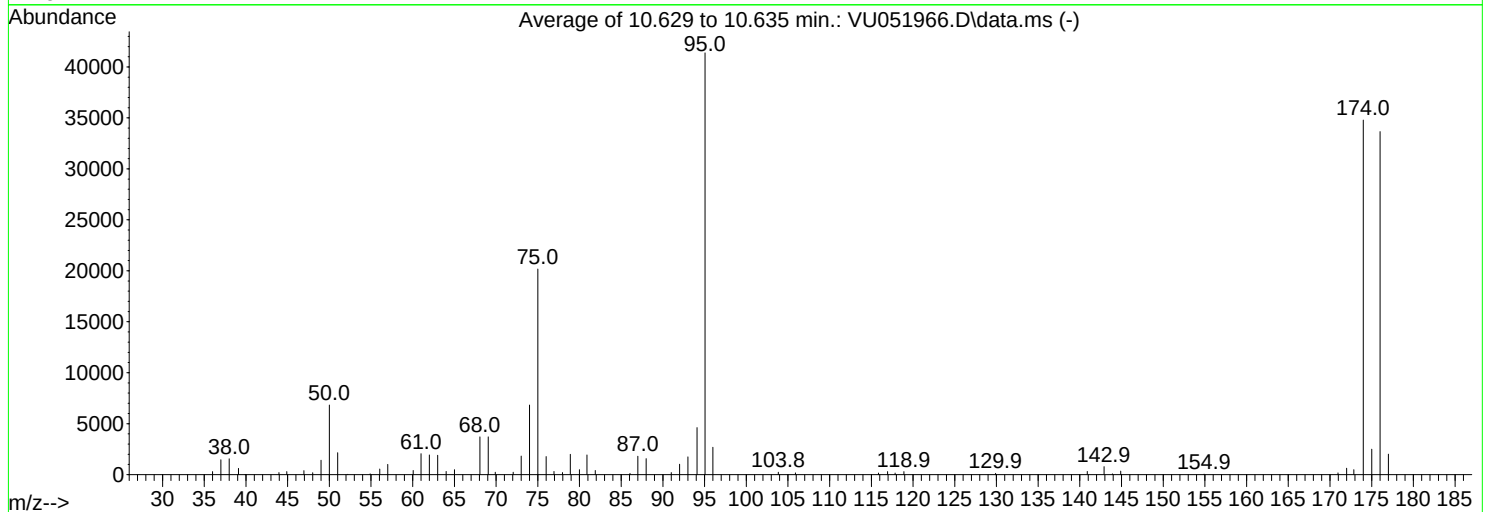


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112022\
Data File : VU051966.D
Acq On : 20 Nov 2022 11:08
Operator : JC/MD
Sample : BFB146
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB146

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Title : VOC Analysis
Last Update : Fri Nov 18 00:53:49 2022

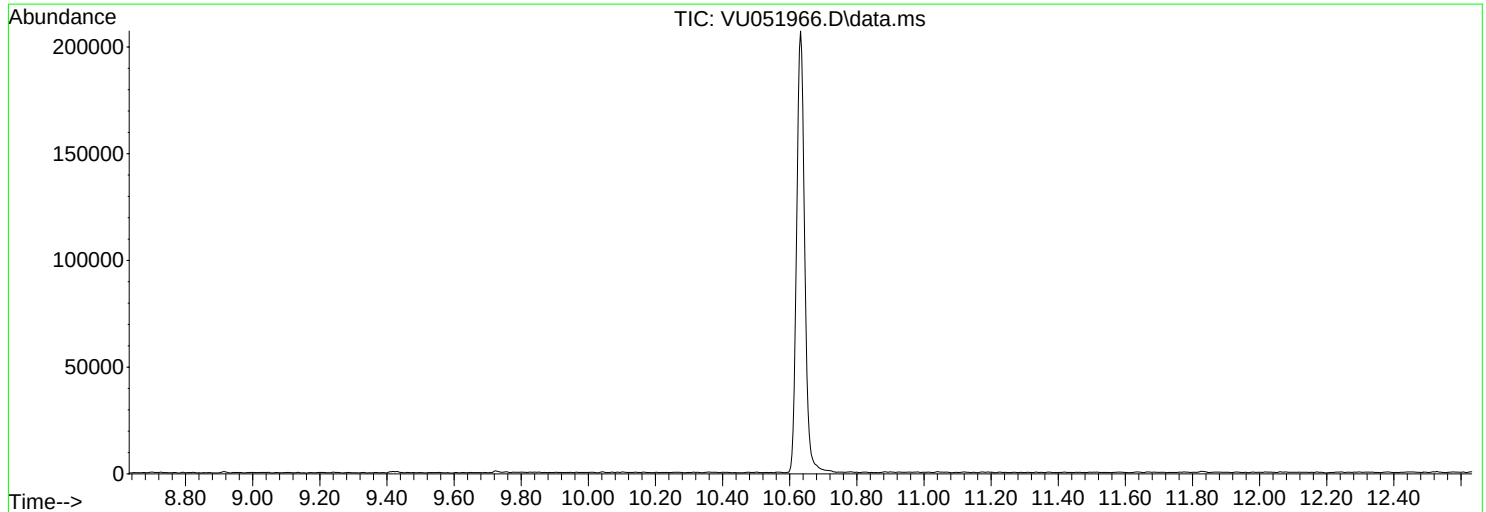

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	6828	PASS
75	95	30	80	48.8	20179	PASS
95	95	100	100	100.0	41384	PASS
96	95	5	9	6.5	2693	PASS
173	174	0.00	2	1.4	483	PASS
174	95	50	120	84.1	34789	PASS
175	174	5	9	7.2	2498	PASS
176	174	95	101	96.7	33651	PASS
177	176	5	9	6.0	2005	PASS

m/z	Abundance
39.90	278.0
43.90	451.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
36.00	289.0
37.00	1505.0
38.00	1520.0
39.10	593.0
39.90	273.0
44.10	545.0
44.90	376.0
46.90	386.0
47.90	204.0
49.00	1417.0
50.00	6689.0
51.00	2144.0
52.20	102.0
56.00	526.0
57.00	1091.0
60.00	323.0
61.00	2009.0
62.00	1967.0
63.00	1772.0
64.00	323.0
65.00	438.0
68.00	3834.0
69.00	3687.0
69.90	293.0
72.00	246.0
73.00	1837.0
74.00	6890.0
75.00	20232.0
76.00	1574.0
77.00	336.0
77.90	190.0
78.90	1910.0
80.00	441.0
80.90	2013.0
81.90	409.0
86.10	131.0
87.00	1682.0
88.00	1520.0
91.00	189.0
92.00	1138.0
93.00	1802.0
94.10	4737.0
95.10	41344.0
96.00	2737.0
103.80	273.0
105.90	195.0
115.90	166.0
116.90	284.0
117.80	194.0
118.90	289.0
129.80	148.0
140.90	324.0
142.90	777.0
143.90	130.0
144.90	309.0
171.00	147.0
172.00	597.0
172.80	479.0
174.00	33632.0
175.00	2428.0
176.00	32760.0
177.00	1926.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
36.00	317.0
37.00	1516.0
38.00	1622.0
39.10	646.0
39.90	267.0
44.00	661.0
44.90	291.0
47.00	415.0
48.00	188.0
49.00	1440.0
50.00	6959.0
51.00	2214.0
54.90	110.0
56.10	577.0
57.00	1017.0
60.10	405.0
61.00	2110.0
62.00	1987.0
63.00	1957.0
64.00	319.0
65.00	521.0
68.00	3742.0
69.10	3788.0
69.90	239.0
72.10	263.0
73.00	1846.0
74.00	7086.0
75.00	20768.0
76.00	1846.0
76.90	318.0
78.00	234.0
78.90	2014.0
80.00	485.0
80.90	2032.0
81.90	417.0
86.10	108.0
87.00	1901.0
88.00	1557.0
91.00	239.0
92.00	1063.0
93.00	1798.0
94.10	4725.0
95.00	42696.0
96.00	2756.0
103.80	237.0
105.90	173.0
115.90	149.0
116.90	293.0
117.80	152.0
118.90	301.0
129.90	122.0
140.90	329.0
142.90	826.0
143.90	104.0
144.90	346.0
171.00	190.0
172.00	634.0
172.90	503.0
174.00	36072.0
175.00	2569.0
176.00	34920.0
177.00	2064.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
36.00	303.0
37.00	1379.0
38.00	1519.0
39.10	597.0
39.90	322.0
44.00	742.0
44.90	212.0
47.00	382.0
48.10	200.0
49.00	1360.0
50.00	6836.0
51.00	2083.0
54.90	127.0
56.00	568.0
57.00	909.0
60.10	505.0
61.00	2057.0
62.00	1820.0
63.00	1992.0
64.00	326.0
65.00	498.0
68.10	3554.0
69.10	3620.0
70.00	168.0
72.10	209.0
73.00	1792.0
74.00	6525.0
75.00	19536.0
76.00	1883.0
76.90	277.0
78.00	210.0
78.90	2057.0
80.00	526.0
80.90	1752.0
81.90	389.0
86.00	124.0
87.00	1833.0
88.00	1642.0
91.00	207.0
92.00	881.0
93.00	1643.0
94.10	4405.0
95.00	40112.0
96.00	2587.0
103.90	182.0
105.90	142.0
115.80	134.0
117.00	316.0
117.90	125.0
118.90	311.0
130.00	130.0
140.90	308.0
142.90	767.0
144.90	375.0
154.90	130.0
170.90	195.0
172.00	674.0
172.90	467.0
174.00	34664.0
175.00	2497.0
176.00	33272.0
177.00	2025.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146