

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112024\
 Data File : VU061878.D
 Acq On : 20 Nov 2024 20:10
 Operator : MD/SY
 Sample : P4885-01DL 10X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3P6DL

Quant Time: Nov 21 01:33:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 21 01:18:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	146138	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	159667	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	61197	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	44048	6.145	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 122.800%	
7) Chloroethane-d5	1.872	69	28038	4.422	ug/L	-0.04
Spiked Amount	5.000	Range	65 - 130	Recovery	= 88.400%	
11) 1,1-Dichloroethene-d2	2.547	65	17894	6.248	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	= 125.000%	
20) 2-Butanone-d5	4.615	46	110765	49.207	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	= 98.420%	
24) Chloroform-d	5.049	84	90059	5.150	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 103.000%	
26) 1,2-Dichloroethane-d4	5.692	65	50158	5.573	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 111.400%	
32) Benzene-d6	5.714	84	171399	5.510	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 110.200%	
36) 1,2-Dichloropropane-d6	6.679	67	58049	5.492	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 109.800%	
41) Toluene-d8	7.888	98	137927	5.316	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 106.400%	
43) trans-1,3-Dichloroprop...	8.174	79	16483	4.212	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 84.200%	
46) 2-Hexanone-d5	8.627	63	87417	48.942	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 97.880%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49891	4.723	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 94.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152	49792	5.502	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 110.000%	
Target Compounds						Qvalue
13) Acetone	2.624	43	15717	10.113	ug/L	95
16) Methylene chloride	3.033	84	3414	0.290	ug/L	98
34) Trichloroethene	6.534	95	4814	0.374	ug/L	95
47) Tetrachloroethene	8.544	164	34869	3.725	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112024\
Data File : VU061878.D
Acq On : 20 Nov 2024 20:10
Operator : MD/SY
Sample : P4885-01DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3P6DL

Quant Time: Nov 21 01:33:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 21 01:18:14 2024
Response via : Initial Calibration

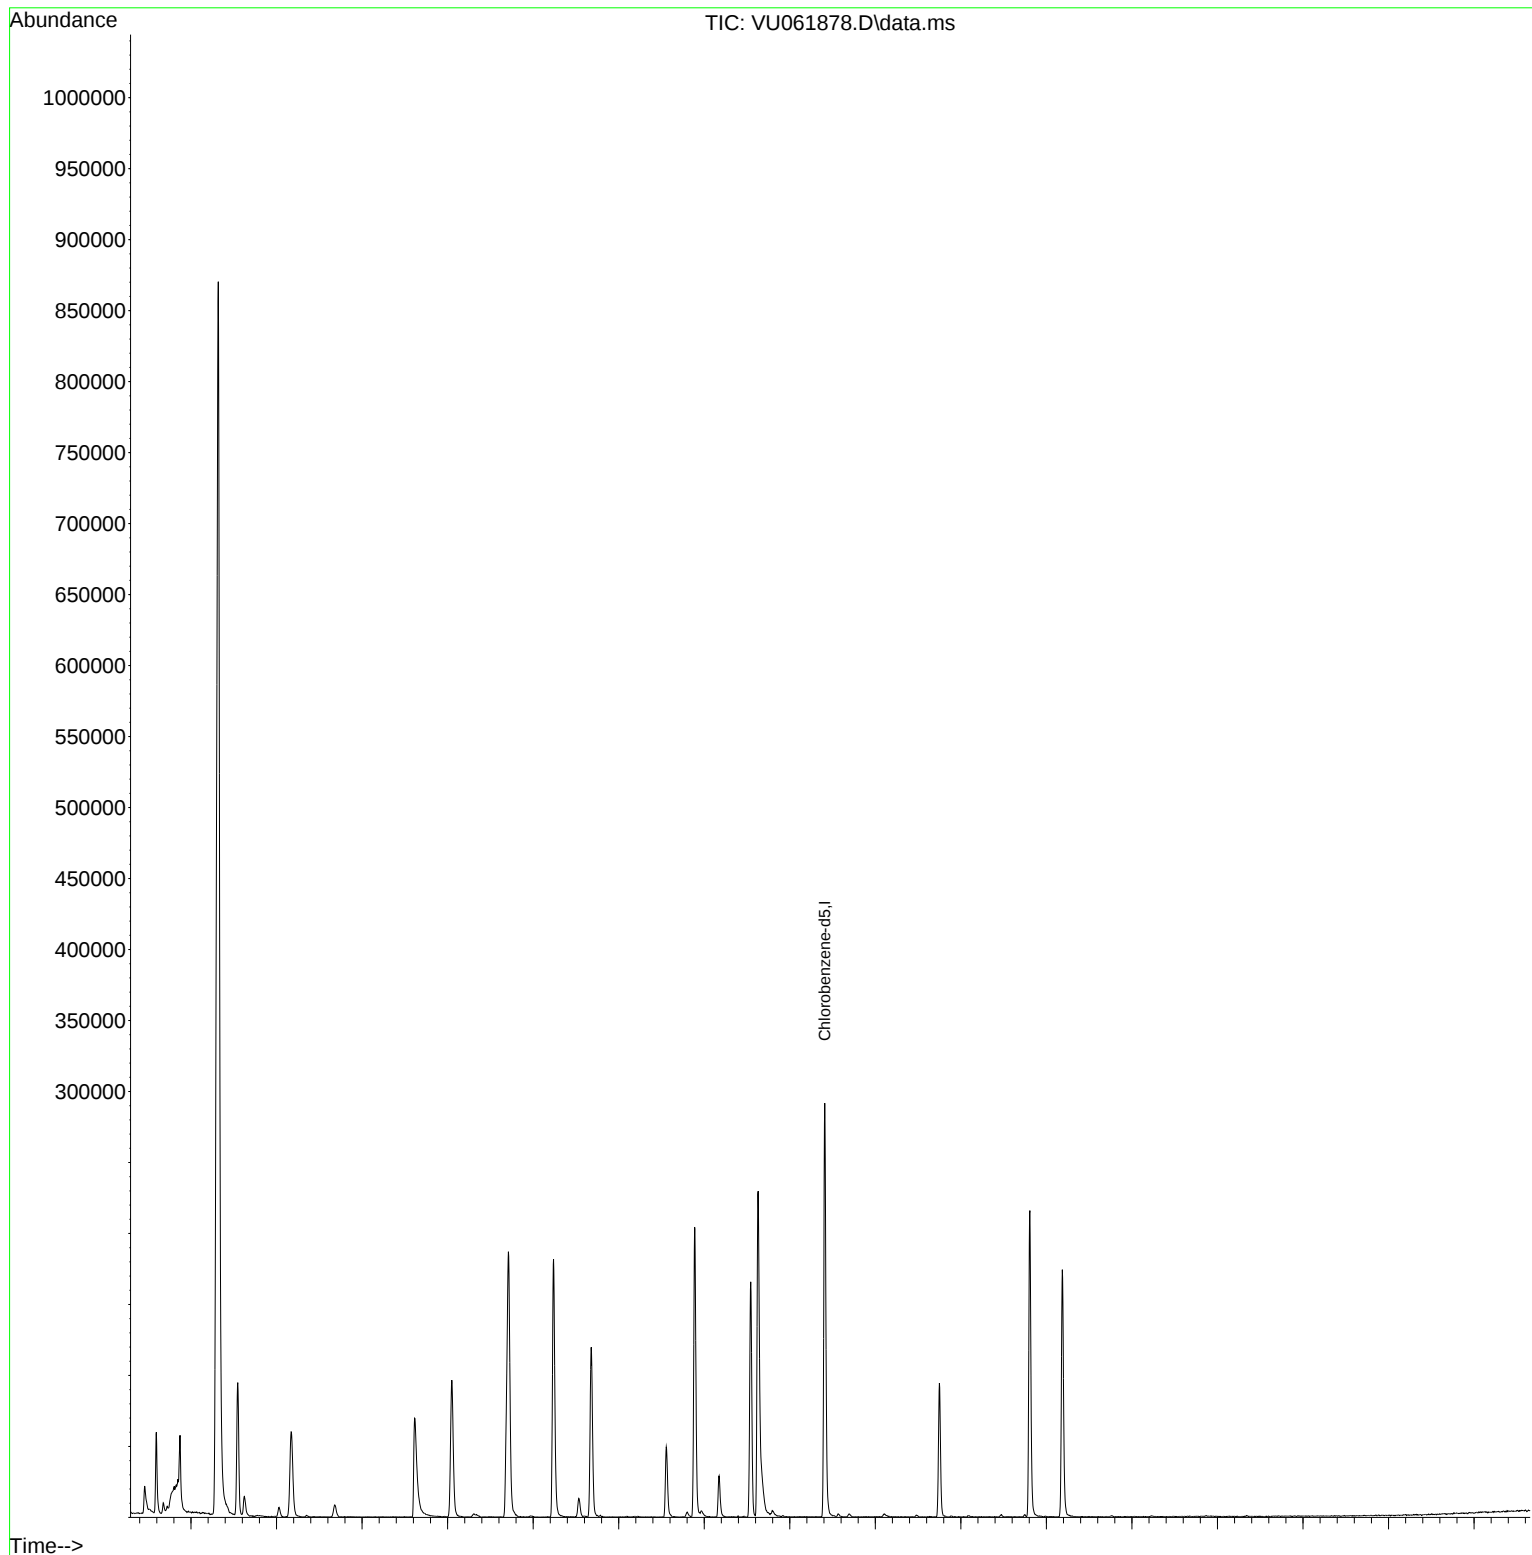

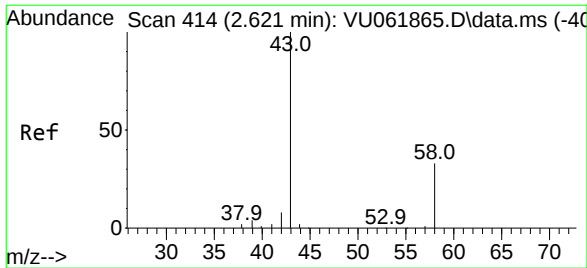

#13

Acetone

Concen: 10.113 ug/L

RT: 2.624 min Scan# 41

Delta R.T. 0.003 min

Lab File: VU061878.D

Acq: 20 Nov 2024 20:10

Instrument :

MSVOA_U

ClientSampleId :





BG3P6DL

Tgt Ion: 43 Resp: 15717

Ion Ratio Lower Upper

43 100

58 34.9 0.0 64.0

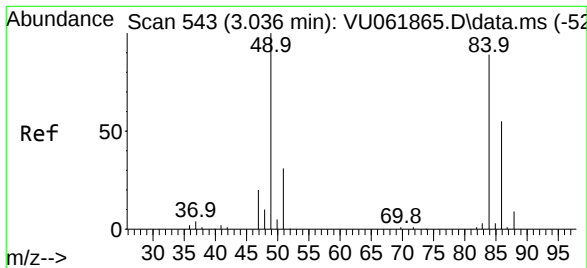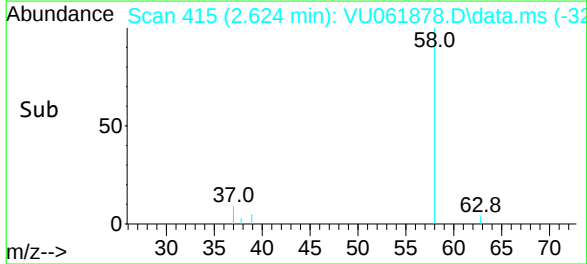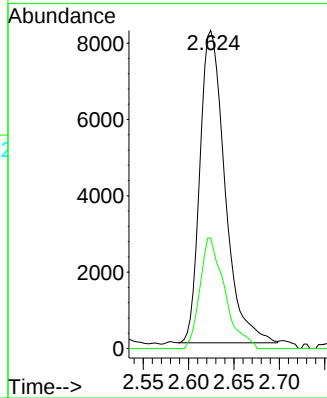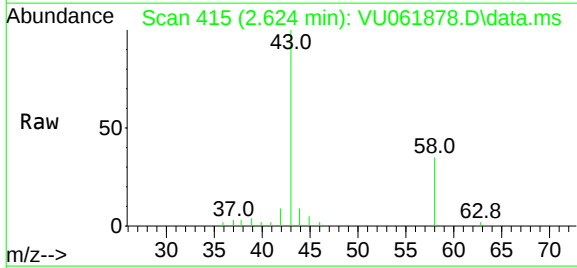

#16

Methylene chloride

Concen: 0.290 ug/L

RT: 3.033 min Scan# 542

Delta R.T. -0.003 min

Lab File: VU061878.D

Acq: 20 Nov 2024 20:10




Tgt Ion: 84 Resp: 3414


Ion Ratio Lower Upper

84 100

86 60.7 43.5 80.7


49 113.9 81.9 152.1

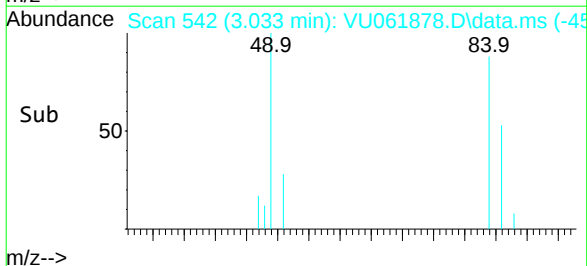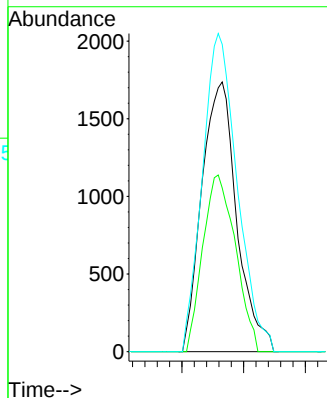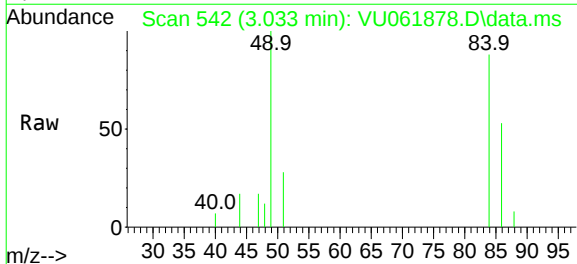

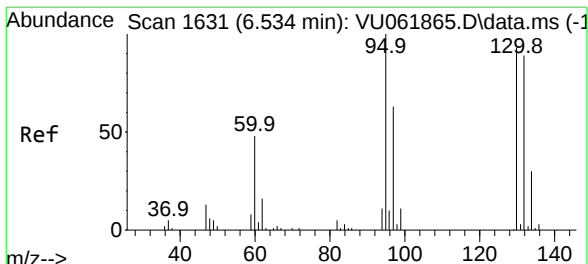




#34
 Trichloroethene
 Concen: 0.374 ug/L
 RT: 6.534 min Scan# 1631
 Delta R.T. -0.000 min
 Lab File: VU061878.D
 Acq: 20 Nov 2024 20:10

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3P6DL

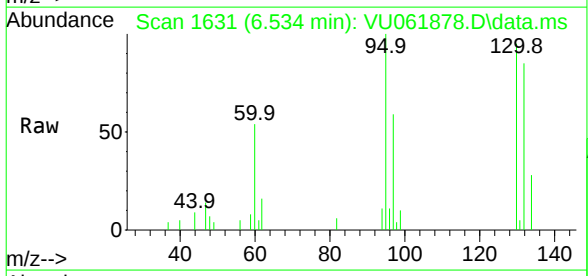

Tgt Ion: 95 Resp: 4814

Ion	Ratio	Lower	Upper
95	100		
97	59.1	45.9	85.3
132	85.5	63.8	118.4
130	94.6	65.5	121.7

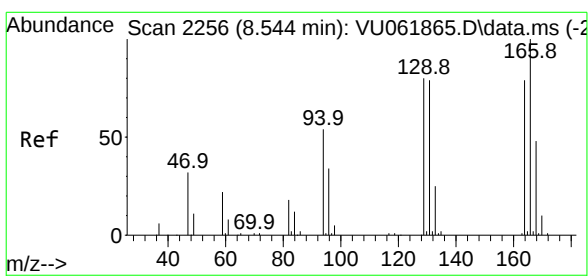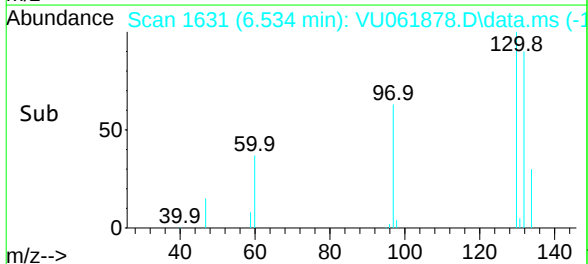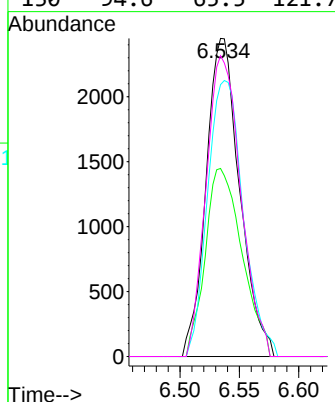

#47
 Tetrachloroethene
 Concen: 3.725 ug/L
 RT: 8.544 min Scan# 2256
 Delta R.T. -0.000 min
 Lab File: VU061878.D
 Acq: 20 Nov 2024 20:10

Tgt Ion: 164 Resp: 34869

Ion	Ratio	Lower	Upper
164	100		
129	103.1	73.2	136.0
131	95.4	72.3	134.3
166	129.7	90.2	167.4

