
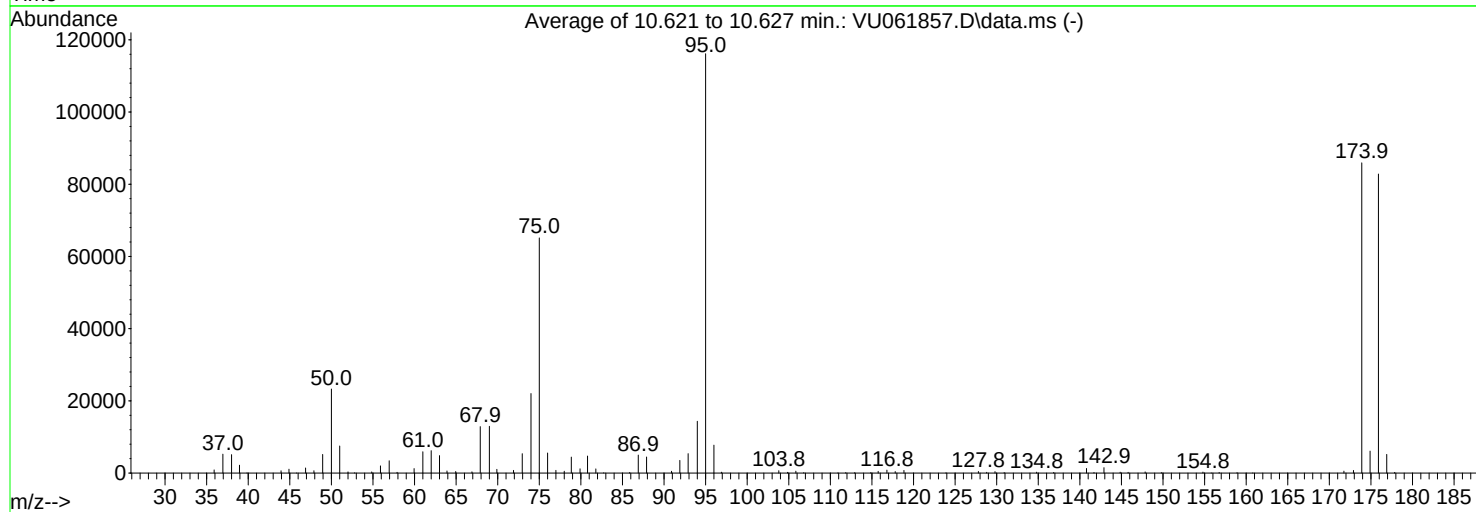


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112024\
Data File : VU061857.D
Acq On : 20 Nov 2024 09:40
Operator : MD/SY
Sample : BFB032
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB032

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 21 03:29:06 2024

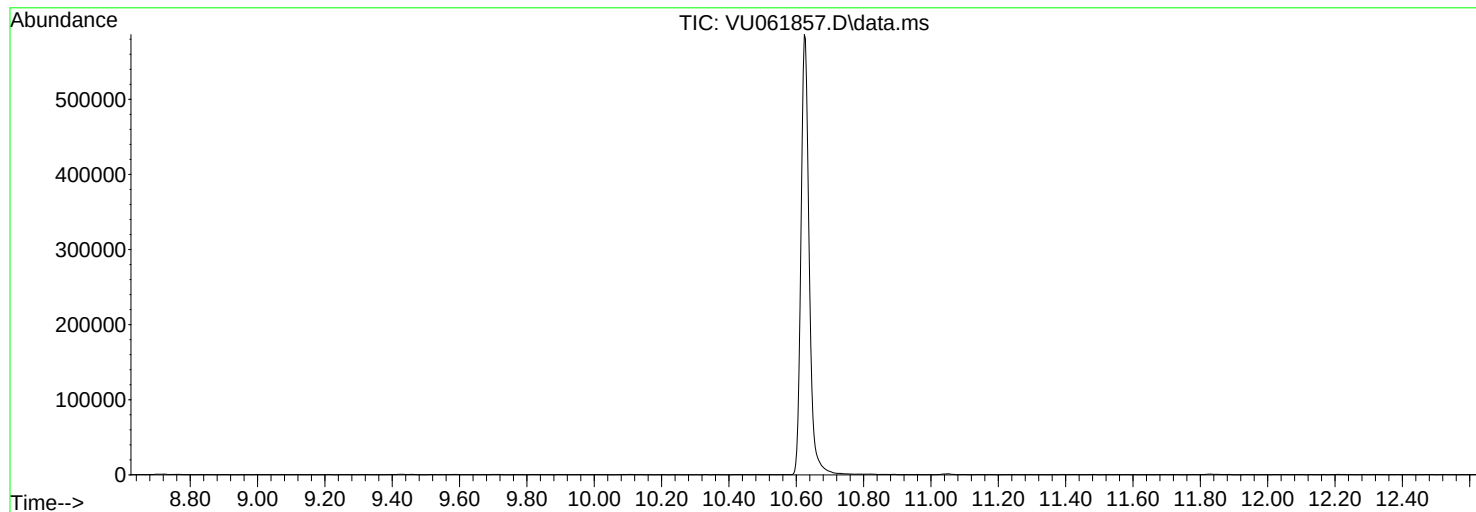

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	23277	PASS
75	95	30	80	56.1	65131	PASS
95	95	100	100	100.0	116147	PASS
96	95	5	9	6.7	7735	PASS
173	174	0.00	2	0.8	729	PASS
174	95	50	120	74.0	85920	PASS
175	174	5	9	7.1	6084	PASS
176	174	95	101	96.4	82824	PASS
177	176	5	9	6.2	5175	PASS

m/z	Abundance
39.80	125.0
44.00	396.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	837.0
37.00	5066.0
38.00	5203.0
39.00	2032.0
40.00	180.0
43.90	1055.0
44.90	1006.0
45.80	104.0
46.90	1510.0
47.90	668.0
49.00	4969.0
50.00	22696.0
51.00	7074.0
52.00	320.0
52.80	131.0
54.90	353.0
55.90	1871.0
57.00	3453.0
57.90	185.0
60.00	1214.0
61.00	5499.0
62.00	6076.0
63.00	4820.0
63.90	543.0
64.90	437.0
66.90	346.0
67.90	12357.0
69.00	12411.0
69.90	1030.0
71.90	665.0
72.90	5141.0
74.00	21168.0
75.00	62264.0
76.00	5526.0
77.00	684.0
78.00	563.0
78.90	4349.0
79.90	1136.0
80.80	4500.0
81.80	1020.0
85.90	136.0
86.90	4736.0
87.90	4101.0
90.90	477.0
91.90	3359.0
92.90	5093.0
94.00	13689.0
95.00	110032.0
96.00	7417.0
96.90	253.0
103.80	660.0
104.90	179.0
105.80	494.0
106.80	110.0
111.90	113.0
114.80	110.0
115.70	420.0
116.80	769.0
117.80	459.0
118.80	688.0
127.80	407.0
128.90	226.0
129.80	415.0
130.90	153.0
134.80	219.0
136.90	162.0
140.80	1266.0
141.60	161.0
142.90	1385.0
144.80	235.0
145.80	162.0
147.80	303.0
149.80	123.0
154.80	230.0
156.80	160.0
171.80	538.0
172.80	672.0
173.90	79184.0
174.90	5524.0
175.90	76560.0
176.90	4903.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	903.0
36.90	5381.0
38.00	5202.0
38.90	2275.0
39.90	169.0
44.00	1050.0
44.90	1108.0
46.90	1463.0
47.90	659.0
49.00	5394.0
50.00	23920.0
51.00	7757.0
52.00	341.0
52.80	118.0
54.90	325.0
55.90	2041.0
56.90	3451.0
57.90	217.0
60.00	1295.0
61.00	6078.0
62.00	6360.0
63.00	5046.0
63.90	622.0
65.00	472.0
66.90	364.0
67.90	13353.0
69.00	13320.0
69.90	1066.0
71.90	808.0
72.90	5482.0
74.00	22760.0
75.00	67568.0
76.00	5688.0
77.00	799.0
78.00	548.0
78.90	4578.0
79.90	1208.0
80.80	4840.0
81.80	1210.0
82.80	105.0
85.80	130.0
86.90	5161.0
87.90	4561.0
90.90	534.0
91.90	3612.0
92.90	5514.0
94.00	14740.0
95.00	119592.0
96.00	7960.0
96.90	253.0
103.80	692.0
104.80	232.0
105.80	544.0
106.80	134.0
111.80	135.0
112.90	126.0
114.80	111.0
115.80	491.0
116.80	834.0
117.80	449.0
118.90	776.0
123.90	104.0
127.80	438.0
128.80	217.0
129.80	420.0
130.90	141.0
134.80	273.0
136.90	189.0
140.80	1307.0
141.70	160.0
142.90	1617.0
144.90	270.0
145.80	233.0
147.80	337.0
149.80	145.0
154.80	312.0
156.80	178.0
158.90	153.0
171.70	559.0
172.90	732.0
173.90	88816.0
174.90	6286.0
175.90	85664.0
176.90	5366.0
177.90	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	893.0
37.00	5282.0
38.00	4940.0
38.90	2245.0
39.90	168.0
43.90	986.0
44.90	1124.0
46.90	1283.0
47.90	639.0
48.90	5124.0
50.00	23216.0
51.00	7683.0
52.00	328.0
54.80	275.0
55.90	2052.0
56.90	3313.0
57.90	242.0
59.90	1251.0
61.00	6144.0
62.00	6193.0
63.00	4661.0
63.90	582.0
65.00	420.0
66.90	326.0
67.90	12922.0
69.00	13100.0
69.90	1016.0
71.90	776.0
73.00	5496.0
74.00	22144.0
75.00	65560.0
76.00	5464.0
77.00	800.0
78.00	442.0
78.80	4374.0
79.90	1195.0
80.80	4840.0
81.80	1250.0
82.70	127.0
85.80	123.0
86.90	5051.0
87.90	4692.0
90.90	535.0
91.90	3574.0
92.90	5567.0
94.00	14605.0
95.00	118816.0
96.00	7829.0
96.90	250.0
103.80	644.0
104.80	246.0
105.90	569.0
106.80	128.0
110.90	134.0
111.80	161.0
112.90	138.0
114.90	102.0
115.80	516.0
116.80	889.0
117.80	383.0
118.90	776.0
123.90	114.0
127.80	485.0
128.70	207.0
129.80	393.0
130.90	135.0
134.80	280.0
136.80	187.0
140.80	1261.0
141.80	160.0
142.90	1529.0
144.90	261.0
145.80	263.0
147.90	350.0
149.80	117.0
154.80	299.0
155.80	117.0
156.70	173.0
158.90	188.0
160.80	107.0
171.70	524.0
173.00	783.0
173.90	89760.0
174.90	6443.0
175.90	86248.0
176.90	5255.0
177.80	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032