
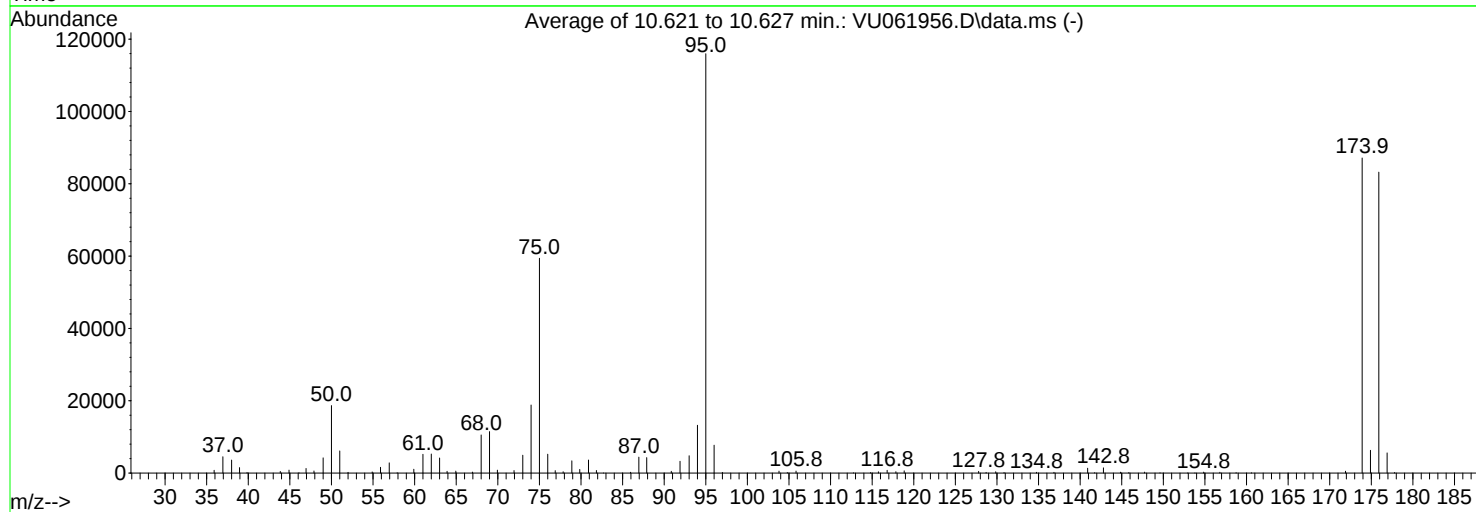


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112224\
Data File : VU061956.D
Acq On : 22 Nov 2024 07:51
Operator : MD/SY
Sample : BFB034
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB034

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 01:25:39 2024

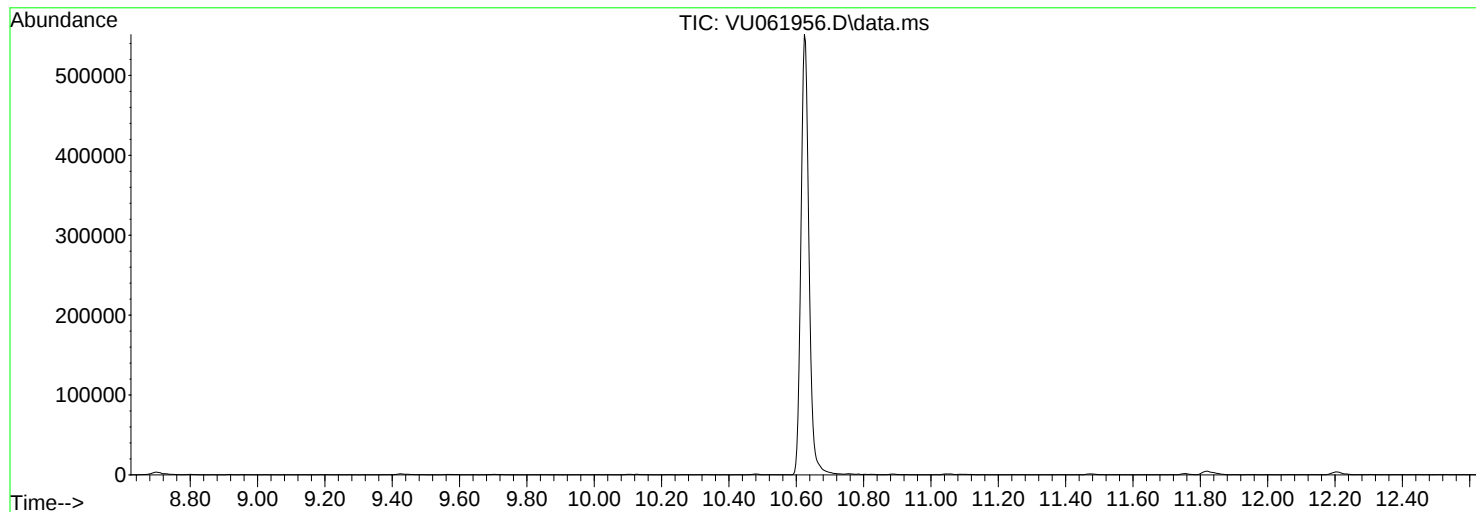

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	18667	PASS
75	95	30	80	51.2	59397	PASS
95	95	100	100	100.0	115968	PASS
96	95	5	9	6.7	7718	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	87128	PASS
175	174	5	9	7.2	6294	PASS
176	174	95	101	95.5	83216	PASS
177	176	5	9	6.7	5572	PASS

m/z	Abundance
43.80	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	768.0
37.00	4257.0
38.00	3532.0
38.90	1476.0
39.90	140.0
43.90	704.0
44.90	772.0
46.10	119.0
46.90	1281.0
47.90	584.0
49.00	4027.0
50.00	17776.0
51.00	5843.0
52.00	173.0
54.90	305.0
55.90	1536.0
56.90	2796.0
57.90	112.0
59.90	1056.0
61.00	4971.0
62.00	5152.0
63.00	4052.0
63.90	506.0
65.00	529.0
67.00	278.0
68.00	10316.0
69.00	11205.0
70.00	851.0
72.00	706.0
73.00	4821.0
74.00	18120.0
75.00	57528.0
76.00	5236.0
76.90	681.0
77.80	370.0
78.90	3240.0
79.90	997.0
80.90	3459.0
81.90	693.0
82.70	102.0
85.90	220.0
86.90	4301.0
87.90	3972.0
90.80	421.0
91.90	3194.0
93.00	4481.0
94.00	12737.0
95.00	110728.0
96.00	7512.0
97.00	171.0
103.80	553.0
104.80	155.0
105.90	598.0
112.80	106.0
114.80	118.0
115.80	336.0
116.80	755.0
117.80	376.0
118.80	604.0
127.80	477.0
128.70	147.0
129.90	319.0
130.90	173.0
134.70	214.0
136.90	206.0
140.90	1346.0
141.80	123.0
142.80	1334.0
144.80	262.0
145.90	123.0
147.80	259.0
152.90	104.0
154.80	287.0
156.80	201.0
158.70	114.0
171.90	452.0
173.90	81064.0
174.90	5823.0
175.90	77632.0
176.90	5260.0
177.80	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	778.0
37.00	4661.0
38.00	3745.0
38.90	1559.0
39.90	154.0
43.90	698.0
44.90	863.0
46.10	116.0
46.90	1348.0
47.90	606.0
49.00	4362.0
50.00	19088.0
51.00	6360.0
52.00	211.0
54.90	352.0
55.90	1663.0
57.00	2914.0
57.90	115.0
59.90	1100.0
61.00	5346.0
62.00	5490.0
63.00	4356.0
63.90	517.0
64.90	555.0
66.90	286.0
68.00	10831.0
69.00	11841.0
70.00	831.0
72.00	702.0
73.00	5046.0
74.00	19440.0
75.00	61448.0
76.00	5351.0
76.90	707.0
77.80	375.0
78.90	3496.0
79.80	1041.0
80.90	3691.0
81.90	750.0
86.00	243.0
87.00	4519.0
87.90	4407.0
90.90	528.0
91.90	3313.0
93.00	4920.0
94.00	13688.0
95.00	119872.0
96.00	7993.0
97.00	181.0
103.80	570.0
104.80	158.0
105.90	597.0
112.70	110.0
114.80	127.0
115.70	364.0
116.80	779.0
117.90	381.0
118.90	633.0
127.80	476.0
128.70	180.0
129.80	397.0
130.80	131.0
134.70	206.0
136.90	225.0
140.90	1387.0
141.80	131.0
142.80	1500.0
144.80	273.0
145.80	145.0
147.80	275.0
149.60	118.0
154.90	274.0
156.80	232.0
158.80	131.0
160.60	116.0
171.90	527.0
173.90	89952.0
174.90	6479.0
175.90	85800.0
176.90	5754.0
177.80	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	745.0
36.90	4650.0
38.00	3536.0
39.00	1521.0
39.80	155.0
43.90	644.0
44.90	856.0
47.00	1214.0
47.90	580.0
49.00	4248.0
50.00	19136.0
51.00	6165.0
52.00	222.0
54.90	313.0
55.90	1576.0
57.00	2788.0
59.90	1016.0
61.00	5260.0
62.00	5191.0
63.00	4118.0
63.90	474.0
64.90	566.0
66.90	289.0
68.00	10479.0
69.00	11375.0
69.90	763.0
71.90	701.0
73.00	4963.0
74.00	18904.0
75.00	59216.0
76.00	5076.0
76.90	653.0
77.90	364.0
78.90	3407.0
79.80	994.0
80.90	3708.0
81.80	702.0
85.90	199.0
87.00	4391.0
87.90	4451.0
90.90	545.0
91.90	3318.0
93.00	4981.0
94.00	13242.0
95.00	117304.0
96.00	7649.0
97.00	186.0
103.80	518.0
104.80	173.0
105.80	507.0
114.80	138.0
115.70	388.0
116.80	757.0
117.90	384.0
118.90	636.0
127.80	441.0
128.70	221.0
129.80	413.0
130.80	138.0
134.80	223.0
136.70	219.0
140.90	1298.0
141.70	125.0
142.80	1530.0
144.90	236.0
145.80	176.0
147.70	261.0
149.60	127.0
153.80	112.0
154.90	247.0
156.80	237.0
158.80	131.0
160.60	112.0
171.90	556.0
173.90	90368.0
174.90	6579.0
175.90	86216.0
176.90	5702.0
177.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034