
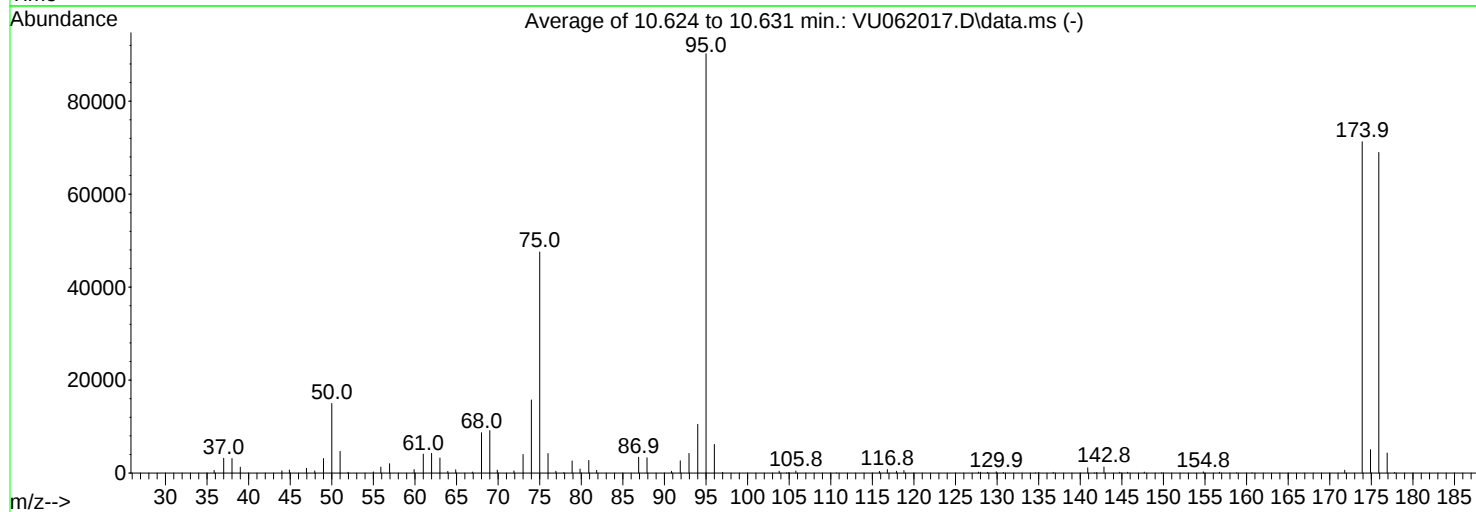


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112524\
Data File : VU062017.D
Acq On : 25 Nov 2024 08:09
Operator : MD/SY
Sample : BFB036
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB036

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 01:25:39 2024

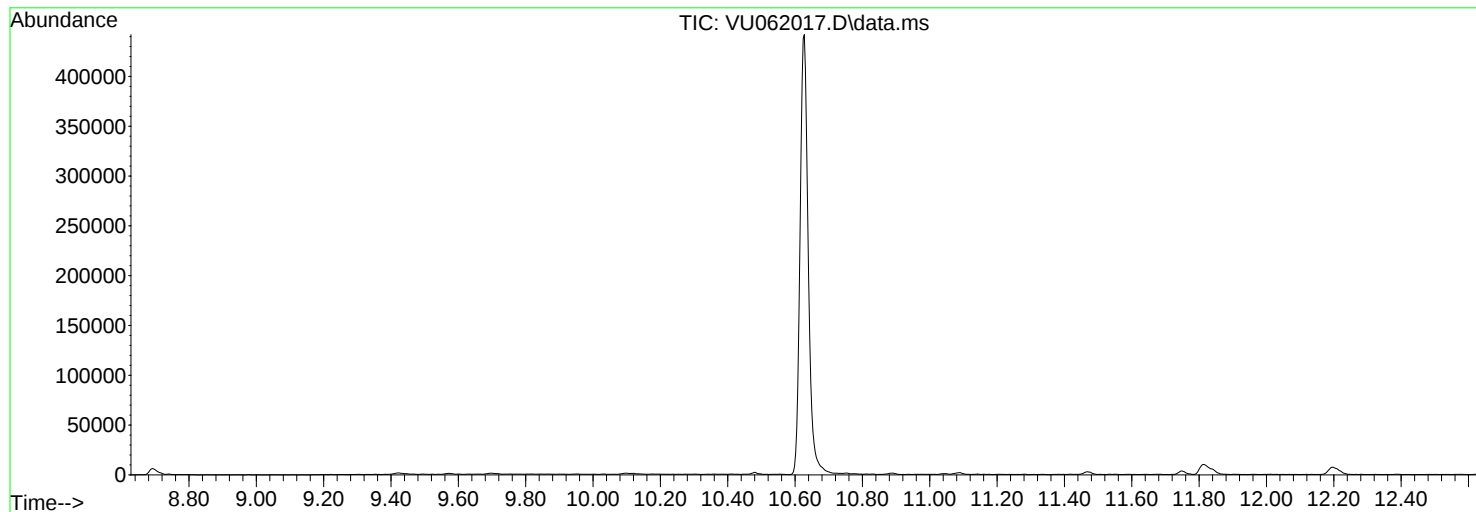

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	14973	PASS
75	95	30	80	52.7	47557	PASS
95	95	100	100	100.0	90208	PASS
96	95	5	9	6.8	6153	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.0	71277	PASS
175	174	5	9	7.1	5036	PASS
176	174	95	101	96.8	68973	PASS
177	176	5	9	6.3	4317	PASS

m/z	Abundance
35.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	901.0
37.00	3294.0
38.00	3215.0
39.00	1333.0
44.00	499.0
44.90	701.0
46.90	1102.0
47.90	500.0
49.00	3230.0
50.00	15509.0
51.00	4929.0
52.00	201.0
55.00	284.0
55.90	1365.0
57.00	2165.0
59.90	833.0
61.00	4244.0
62.00	4301.0
63.00	3271.0
63.90	327.0
64.90	746.0
66.90	222.0
68.00	8992.0
69.00	9564.0
69.90	663.0
71.00	492.0
73.00	3986.0
74.00	16153.0
75.00	48976.0
76.00	4412.0
77.00	441.0
77.90	270.0
78.90	2731.0
79.80	866.0
80.90	2711.0
81.90	614.0
86.90	3409.0
87.90	3452.0
90.80	383.0
91.90	2638.0
93.00	4429.0
94.00	10982.0
95.00	92584.0
96.00	6321.0
97.00	170.0
103.80	476.0
104.70	164.0
105.80	440.0
115.80	397.0
116.80	753.0
117.90	427.0
118.80	579.0
127.80	340.0
128.80	163.0
129.90	332.0
130.70	121.0
134.60	121.0
135.10	140.0
136.80	147.0
140.90	1134.0
142.00	167.0
142.80	1257.0
144.70	196.0
145.70	201.0
147.70	215.0
149.80	139.0
154.80	242.0
156.80	186.0
171.80	588.0
173.90	71920.0
174.90	5223.0
175.90	68744.0
176.90	4383.0
177.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	921.0
37.00	3264.0
38.00	3236.0
39.00	1325.0
44.00	519.0
44.90	719.0
46.90	1113.0
47.90	468.0
49.00	3205.0
50.00	15347.0
51.00	4785.0
52.00	159.0
55.00	271.0
55.90	1347.0
56.90	2091.0
59.90	778.0
61.00	4216.0
62.00	4444.0
63.00	3306.0
64.00	388.0
64.90	737.0
66.90	240.0
68.00	8964.0
69.00	9475.0
69.90	670.0
71.90	517.0
73.00	4094.0
74.00	16110.0
75.00	49032.0
76.00	4336.0
77.00	402.0
78.90	2702.0
79.90	914.0
80.90	2813.0
81.80	615.0
86.90	3514.0
87.90	3456.0
90.80	394.0
91.90	2735.0
92.90	4395.0
94.00	10826.0
95.00	92768.0
96.00	6333.0
97.00	154.0
103.80	439.0
104.90	149.0
105.80	470.0
110.70	101.0
115.90	376.0
116.80	792.0
117.90	402.0
118.80	578.0
127.70	303.0
128.00	297.0
128.90	167.0
129.90	314.0
130.80	130.0
135.00	137.0
136.70	169.0
140.90	1158.0
141.90	156.0
142.80	1367.0
144.70	203.0
145.70	170.0
147.70	226.0
149.80	114.0
154.80	289.0
156.80	189.0
158.80	104.0
160.70	121.0
171.80	647.0
173.90	73288.0
174.90	5130.0
175.90	71248.0
176.90	4436.0
177.80	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	877.0
37.00	3039.0
38.00	2921.0
39.00	1165.0
44.00	482.0
44.90	611.0
47.00	887.0
48.00	442.0
49.00	2927.0
50.00	14063.0
51.00	4312.0
51.90	158.0
55.00	230.0
55.90	1163.0
57.00	1836.0
59.90	695.0
61.00	3811.0
62.00	3992.0
63.00	3164.0
64.00	410.0
64.90	646.0
66.90	222.0
68.00	8092.0
69.00	8459.0
69.90	593.0
71.00	437.0
73.00	3949.0
74.00	14919.0
75.00	44664.0
76.00	3892.0
76.90	363.0
78.90	2416.0
79.90	851.0
80.90	2649.0
81.80	552.0
86.90	3276.0
87.90	2993.0
90.90	379.0
91.90	2558.0
92.90	3885.0
94.00	9688.0
95.00	85272.0
96.00	5804.0
97.00	142.0
103.80	374.0
105.00	168.0
105.80	445.0
115.90	363.0
116.80	762.0
117.90	368.0
118.80	528.0
128.00	272.0
128.90	169.0
129.90	249.0
130.80	124.0
134.90	127.0
136.70	191.0
140.90	1119.0
141.70	147.0
142.90	1341.0
144.80	169.0
145.70	164.0
147.70	202.0
154.80	281.0
156.70	184.0
158.80	121.0
160.60	114.0
171.80	640.0
173.90	68624.0
174.90	4755.0
175.90	66928.0
176.90	4133.0
177.80	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036